


MM421+100uLPh2Por  
4PROTON CDC13 C:\ nsalam 45

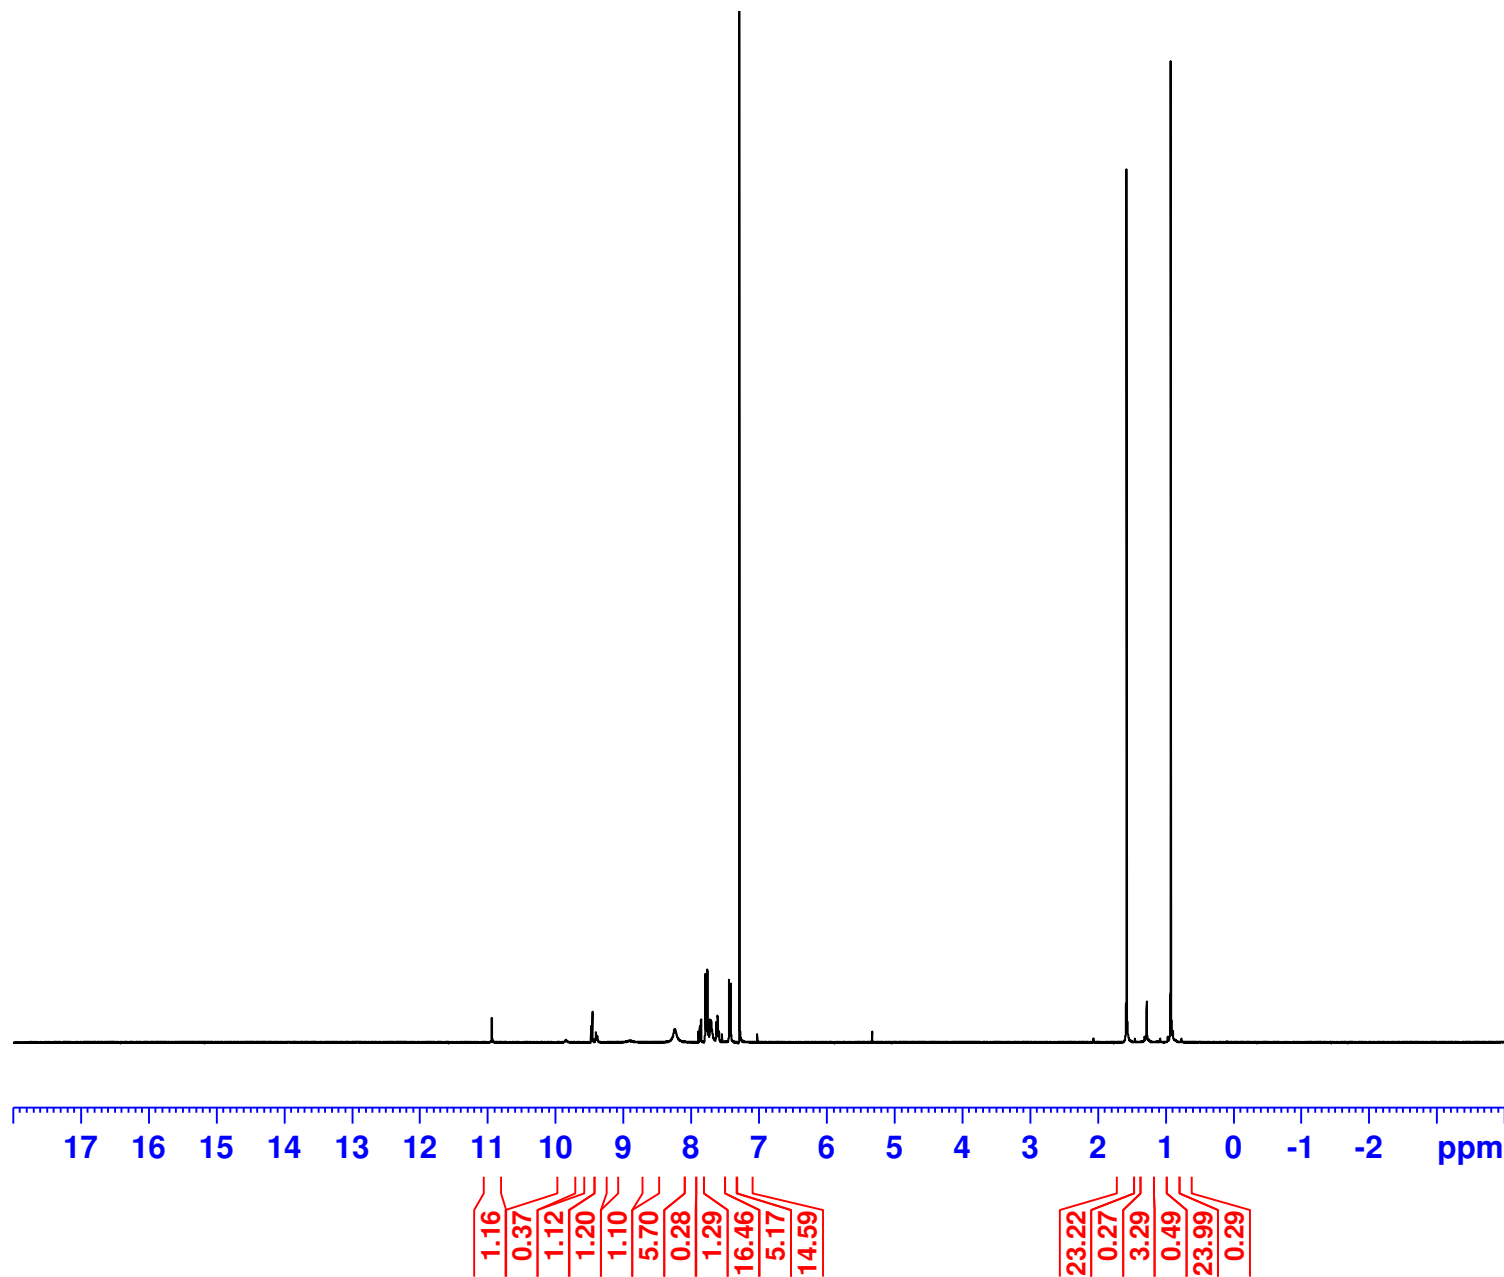

Current Data Parameters  
NAME MANS266\_MM421-Ph2Por\_titration  
EXPNO 28  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20230925  
Time 14.54  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zg30  
TD 98304  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 8802.817 Hz  
FIDRES 0.089547 Hz  
AQ 5.5836673 sec  
RG 206.06  
DW 56.800 usec  
DE 6.50 usec  
TE 295.2 K  
D1 0.20000000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 400.0328002 MHz  
NUC1 1H  
P1 9.45 usec  
PLW1 20.00000000 W

F2 - Processing parameters  
SI 131072  
SF 400.0300000 MHz  
WDW EM  
SSB 0  
LB 0.10 Hz  
GB 0  
PC 1.00