


MM421+400uLPh2Por
4PROTON CDC13 C:\ nsalam 45

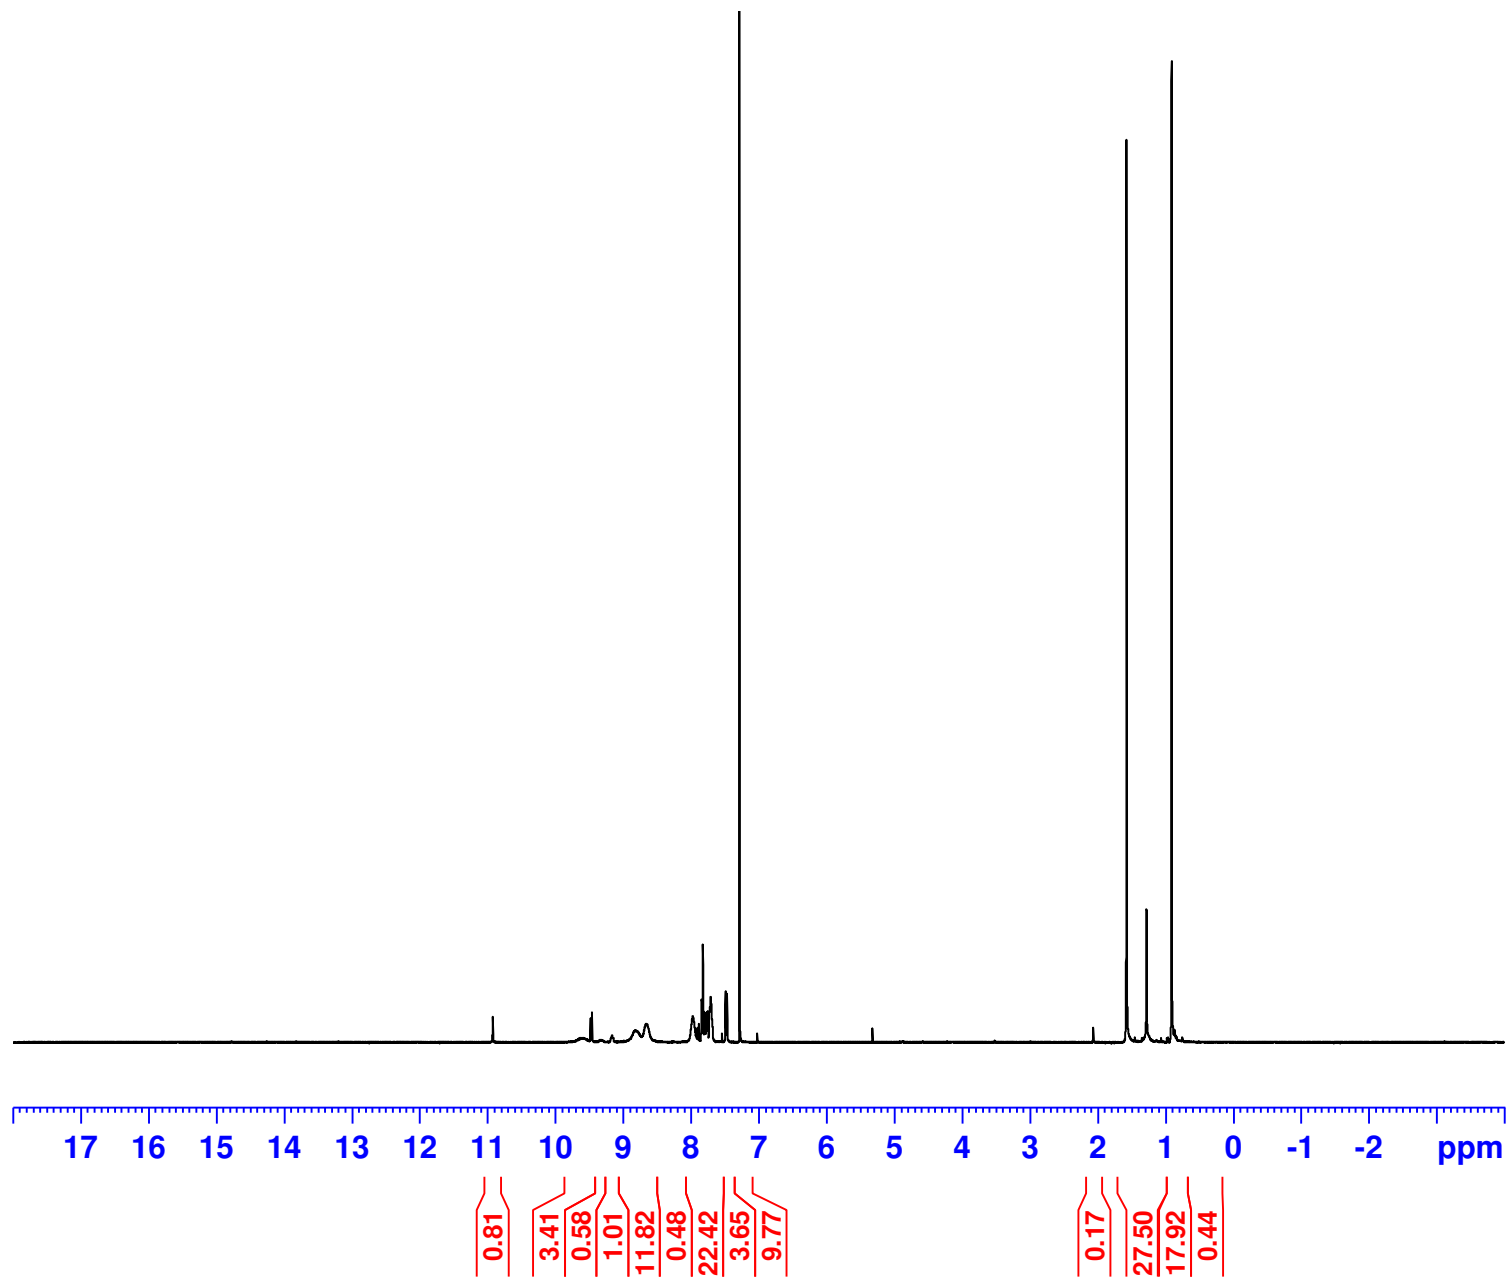

Current Data Parameters
NAME MANS266_MM421-Ph2Por_titration
EXPNO 34
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230925
Time 15.50
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 98304
SOLVENT CDC13
NS 32
DS 2
SWH 8802.817 Hz
FIDRES 0.089547 Hz
AQ 5.5836673 sec
RG 206.06
DW 56.800 usec
DE 6.50 usec
TE 295.2 K
D1 0.20000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 400.0328002 MHz
NUC1 1H
P1 9.45 usec
PLW1 20.00000000 W

F2 - Processing parameters
SI 131072
SF 400.0300000 MHz
WDW EM
SSB 0
LB 0.10 Hz
GB 0
PC 1.00