




Current Data Parameters  
NAME DM24-144  
EXPNO 11  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20240611  
Time 17.24 h  
INSTRUM Avance Neo 400  
PROBHD Z175272\_0007 (  
PULPROG zg30  
TD 32768  
SOLVENT CDCl3  
NS 32  
DS 0  
SWH 6578.947 Hz  
FIDRES 0.401547 Hz  
AQ 2.4903679 sec  
RG 101  
DW 76.000 usec  
DE 7.79 usec  
TE 298.0 K  
D1 2.00000000 sec  
TD0 1  
SFO1 400.1330415 MHz  
NUC1 1H  
P0 3.33 usec  
P1 10.00 usec  
PLW1 20.07200050 W

F2 - Processing parameters  
SI 65536  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0 Hz  
GB 0  
PC 1.00

7.24  
7.24  
7.23  
7.22  
7.21

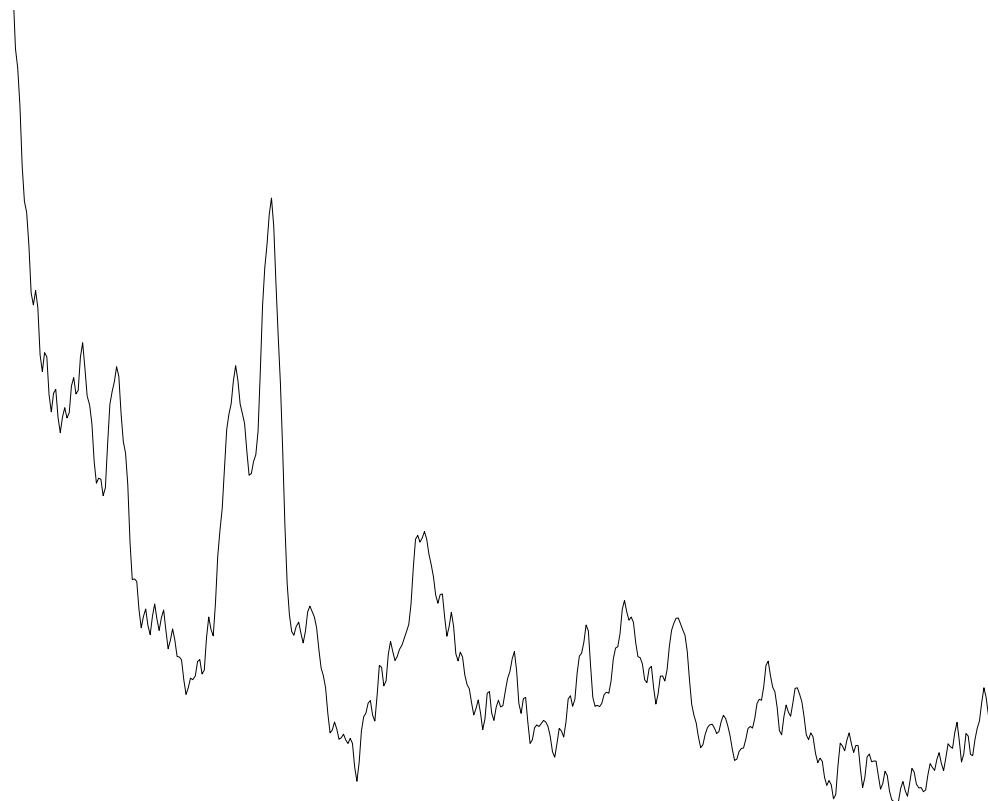

7.26 7.24 7.22 7.20 7.18 7.16 7.14 7.12 ppm