


SR Analyzer (SRA) - TPH IR Analysis - V6.0.21

Sample ID: OTHR477491 Acq. Type: TPH Weight: 33.8 Crucible: 6
Depth: Lithology: Other Sample Type: Core
Acq. Date: February 21 2009 / 3:03:22 AM

Data: C:\Program Files\Thermal Station\Data\320T_A\OTHR477491.RAW
Method: C:\Program Files\Thermal Station\toc_580.PAR
Sequence: C:\Program Files\Thermal Station\Data\Test Drive2\320T_A.pas
Method Information: Initial Temp: 340 °C -- Initial Time: 3 -- Rate : 25.0 °C/Min -- Final Temp: 640 °C -- Final Time: 3 Min -- OxiPurge: 5 Min -- OxiTime: 20 Min -- OxiTemp: 580 °C
FID Temp: 350 °C
FID Gain: Low (10^6)

Calibration Standard Information: Standard Name: 99986 tTemp: 457.0 °C pTPH (S2): 8.41 mg/g S3: 0.39 mg/g S4: 23.99 mg/g
Operator: fujine Instrument name: SRA

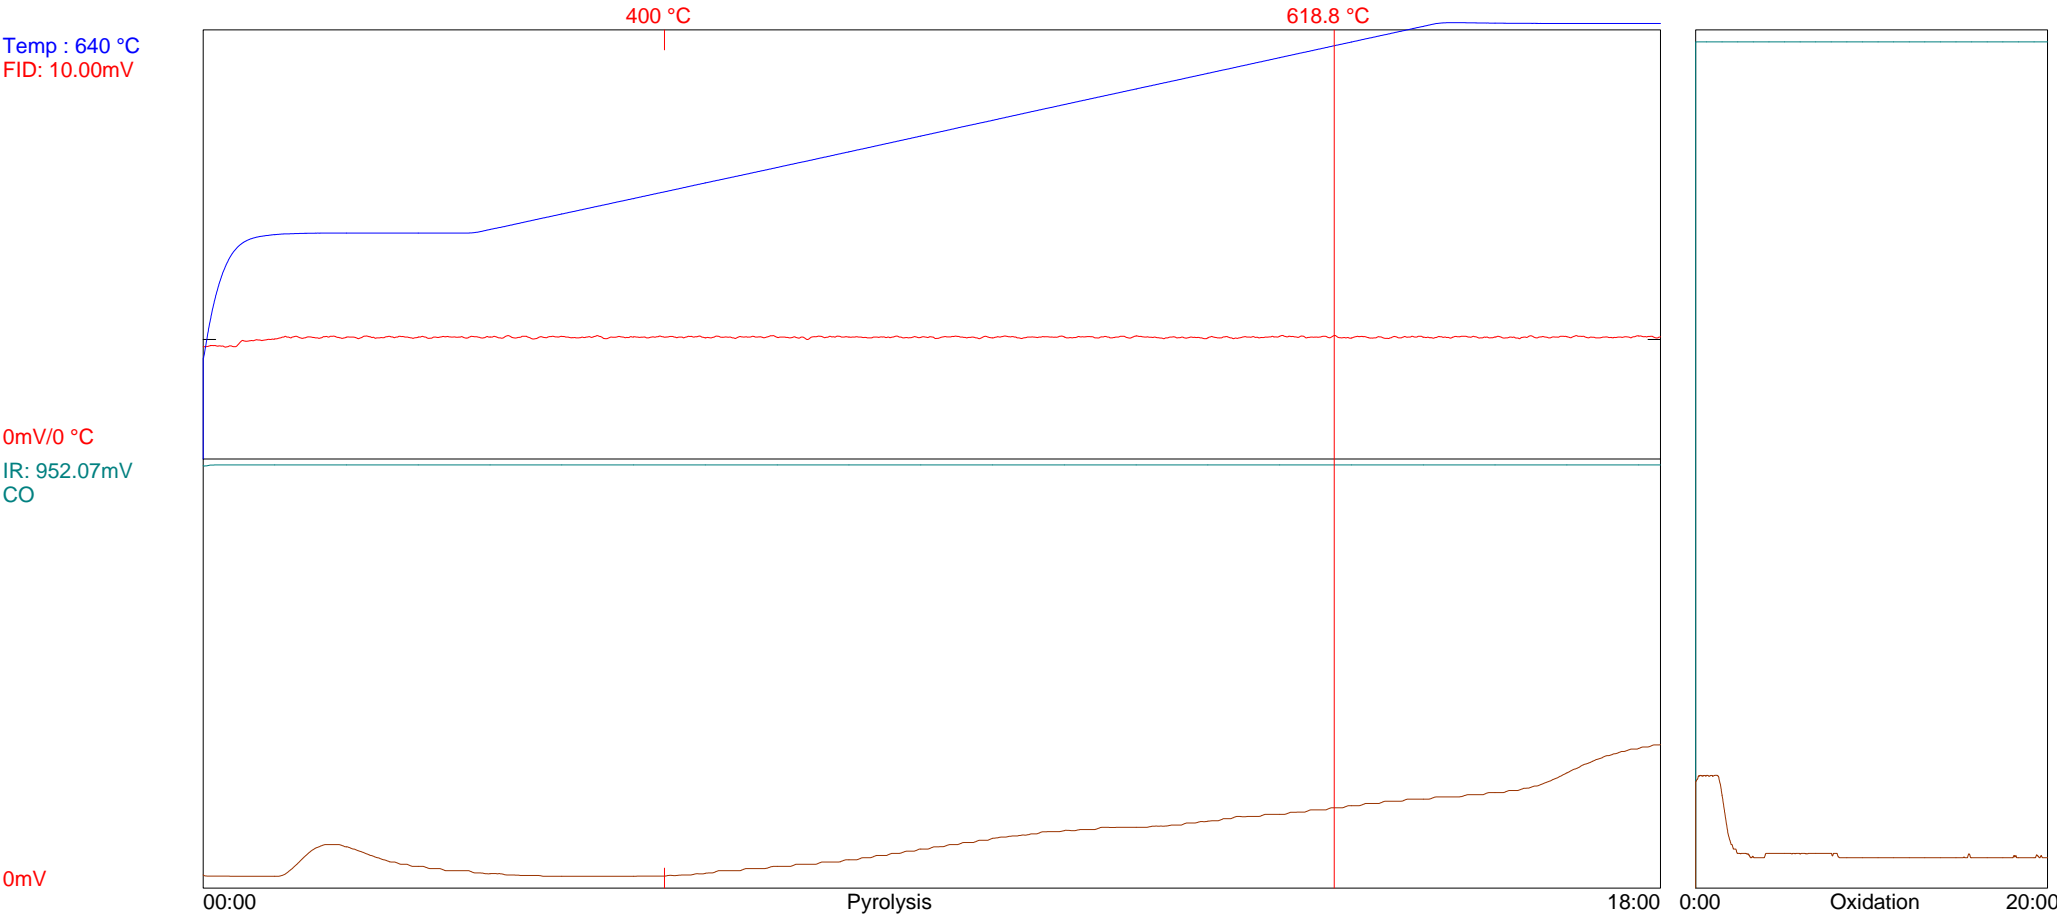

vTPH (S1): .01 mg/g -- pTPH (S2): .12 mg/g -- cTemp(Tmax): 579.8 °C -- tTemp: 618.8 °C -- S3: .65 mg/g -- TOC: 0.83 % -- HI: 15 -- OI: 78 -- PI: 0.04 -- S1/TOC: 0.01