

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\pClKCy000001.d
Method Tune_low_pos.m
Sample Name pClKCy
Comment

Acquisition Date 2018-02-15 16:40:06

Operator Carin Larsson
Instrument / Ser# microTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

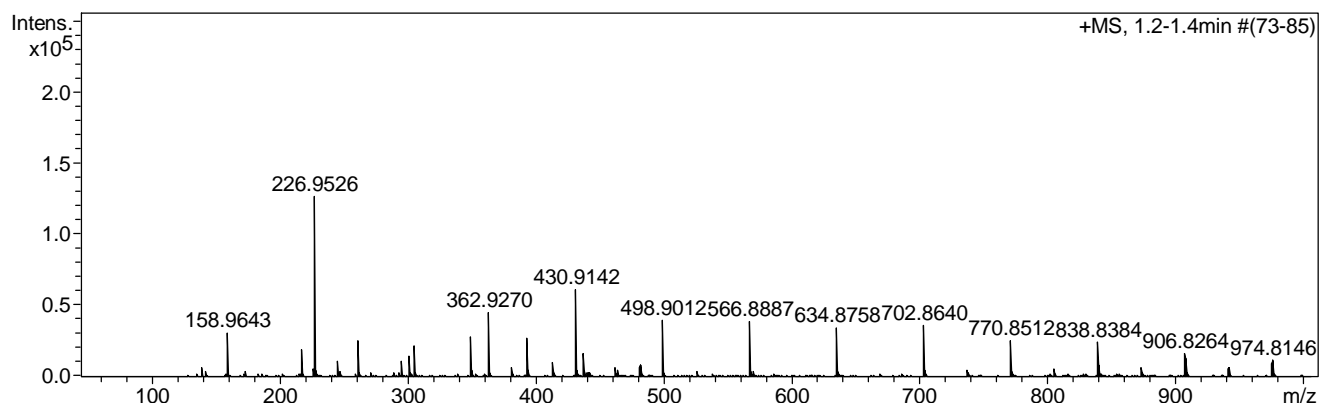

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻	Conf	N-Rule
245.0714	1	C 13 H 15 Cl Na O	100.00	245.0704	-1.0	-4.1	21.7	5.5	even		ok
	2	C 9 H 15 Cl N 5 O	0.00	244.0960	-975.4	-3980.1	691.4	4.5	even		ok