

# Mass Spectrum SmartFormula Report

## Analysis Info


Analysis Name E:\Data2\Kilian\CSA-1-053000001.d  
Method Tune\_low\_pos.m  
Sample Name nicoKthz  
Comment

Acquisition Date 2018-06-13 16:48:16

Operator Carin Larsson  
Instrument / Ser# micrOTOF 125

## Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

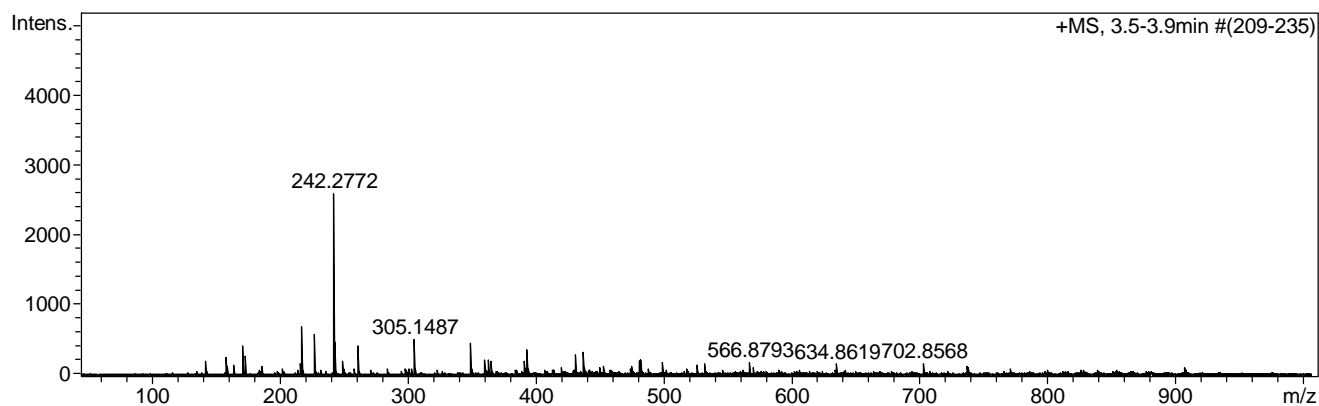

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e <sup>-</sup>	Conf	N-Rule
191.0263	1	C <sub>9</sub> H <sub>7</sub> N <sub>2</sub> O <sub>2</sub> S		191.0274	1.1	5.5	n.a.	7.5	even		ok
212.9990	1	C <sub>9</sub> H <sub>6</sub> N <sub>2</sub> NaO <sub>2</sub> S		213.0093	10.3	48.4	n.a.	7.5	even		ok