

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\CSA-1-054000001.d
Method Tune_low_pos.m
Sample Name oOHKmorpho
Comment

Acquisition Date 2018-06-13 17:00:21

Operator Carin Larsson
Instrument / Ser# micrOTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

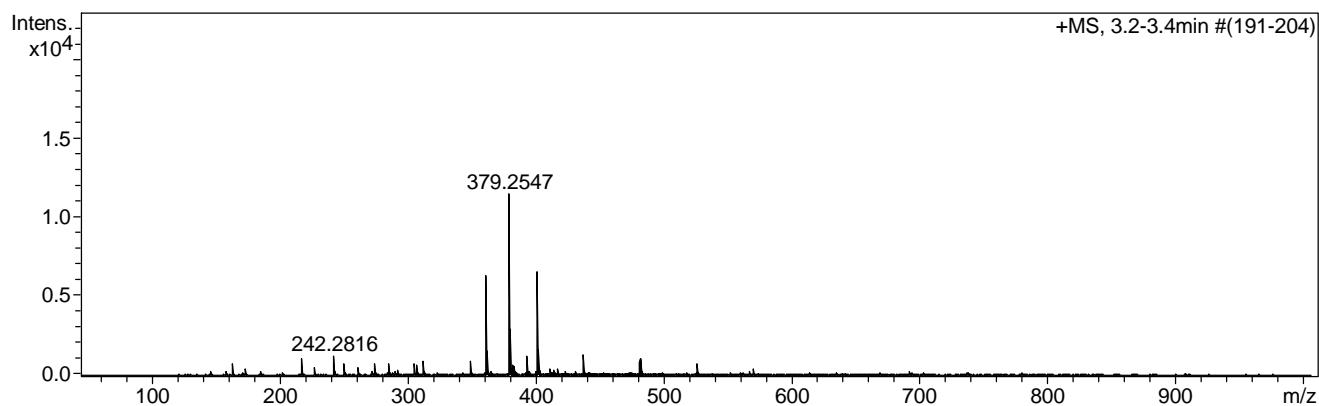

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻	Conf	N-Rule
250.1427	1	C 14 H 20 N O 3	100.00	250.1438	1.1	4.5	20.5	5.5	even		ok