

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\CSA-1-077rerere000001.d
Method Tune_low_pos.m
Sample Name dichlokmanil
Comment

Acquisition Date 2019-02-07 11:11:27

Operator Carin Larsson
Instrument / Ser# microTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

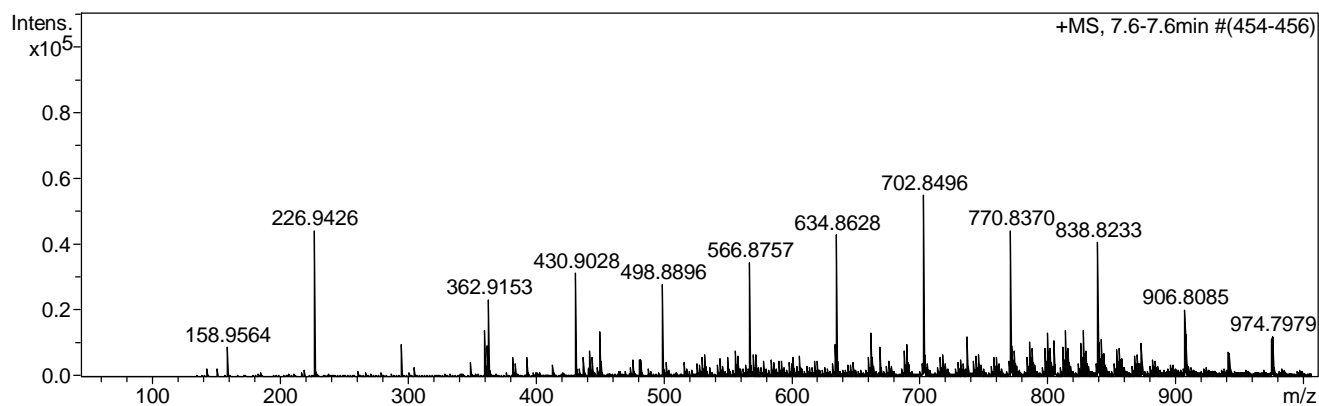

Meas. m/z	#	Formula	Score	m/z	err [mD a]	err [ppm]	mSigm a	rdb	e ⁻ Conf	N-R ule
288.9905	1	C 12 H 8 Cl 2 N 2 Na O	100.00	288.9906	0.1	0.3	297.5	8.5	even	ok