

# Mass Spectrum SmartFormula Report

## Analysis Info


Analysis Name E:\Data2\Kilian\KC-10-072000001.d  
Method Tune\_low\_pos.m  
Sample Name pBrKipr  
Comment

Acquisition Date 2019-02-06 15:04:28

Operator Carin Larsson  
Instrument / Ser# microTOF 125

## Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

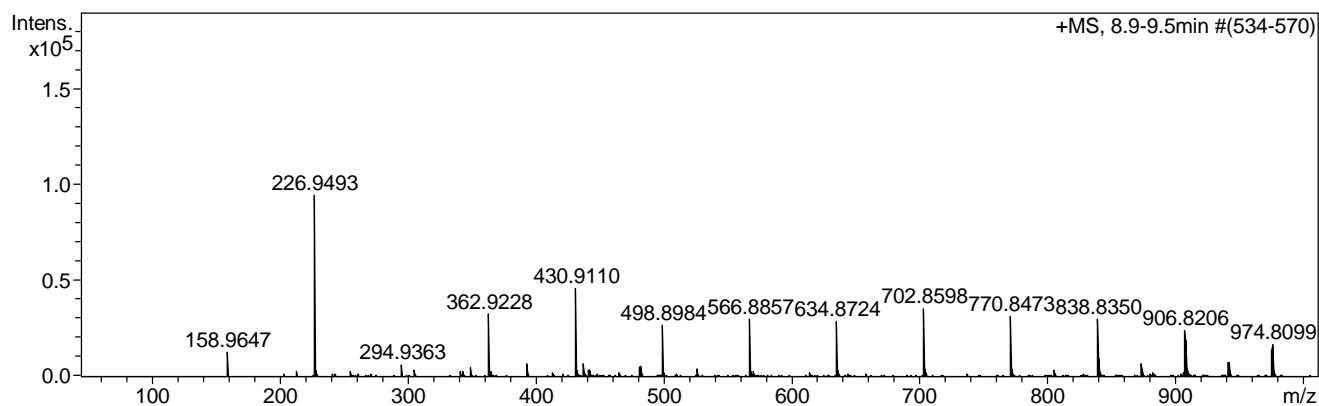

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e <sup>-</sup>	Conf	N-Rule
248.9877	1	C 10 H 11 Br Na O	100.00	248.9885	0.9	3.5	221.3	4.5	even		ok
	2	C 6 H 11 Br N 5 O	0.00	248.0141	-973.5	-3910.0	852.2	3.5	even		ok