

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\KC-Npclean000001.d
Method Tune_low_pos.m
Sample Name KC-NPclean
Comment

Acquisition Date 2019-02-06 16:13:16

Operator Carin Larsson
Instrument / Ser# microTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

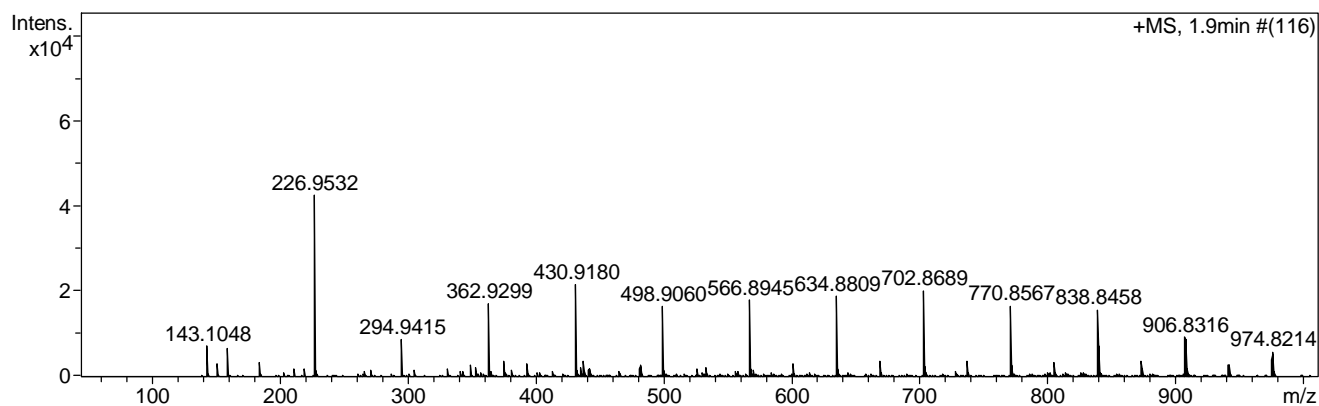

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻	Conf	N-Rule
271.0728	1	C 17 H 12 Na O 2	100.00	271.0730	0.2	0.7	29.4	11.5	even		ok
	2	C 13 H 12 N 5 O 2	0.00	270.0986	-974.2	-3593.9	92.3	10.5	even		ok