

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\CSA-1-48000001.d
Method Tune_low_pos.m
Sample Name mOHKpenten
Comment

Acquisition Date 2018-06-12 17:42:02

Operator Carin Larsson
Instrument / Ser# microTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

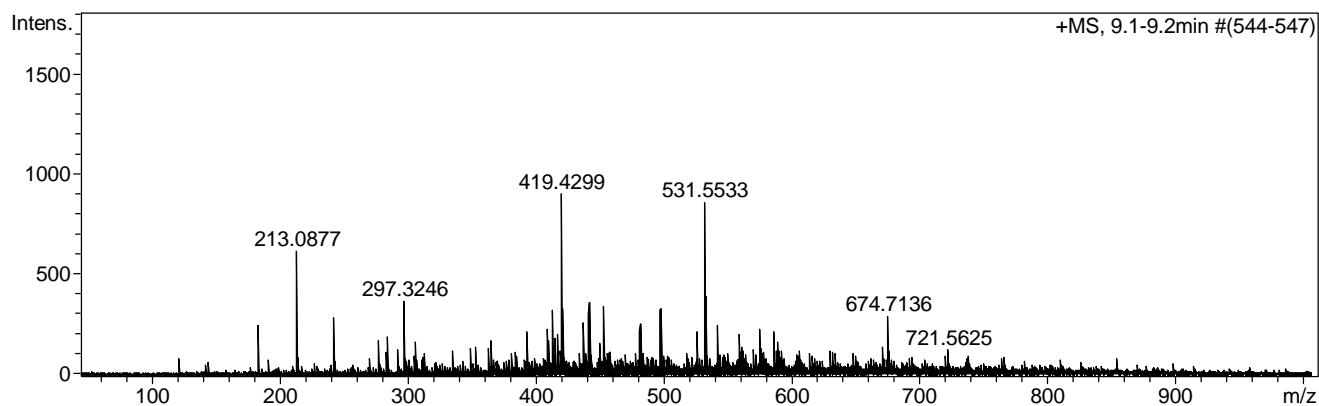

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻	Conf	N-Rule
213.0877	1	C 5 H 14 N 6 Na O 2	0.00	213.1070	19.3	90.6	44.1	1.5	even		ok
	2	C 12 H 14 Na O 2	100.00	213.0886	0.9	4.1	75.2	5.5	even		ok