

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\CSA-1-077rerere000002.d
Method Tune_low_neg.m
Sample Name dichlokmanil
Comment

Acquisition Date 2019-02-07 11:22:11

Operator Carin Larsson
Instrument / Ser# micrOTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4000 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Waste

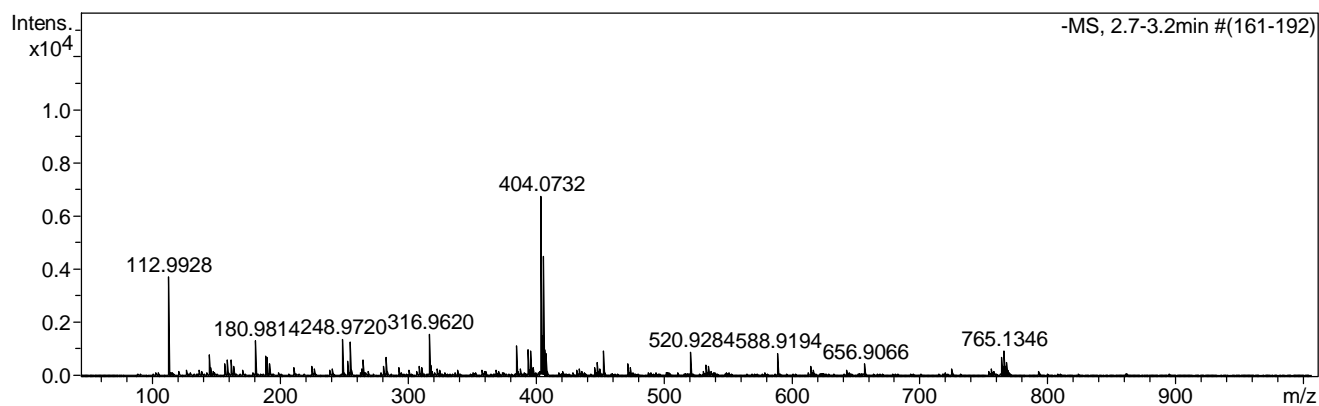

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻ Conf	N-Rule
263.0694	1	C 8 H 10 F 3 N 6 O	0.00	263.0874	17.9	68.1	62.8	5.5	even	ok
	2	C 9 H 11 F 3 N 5 O	0.00	262.0921	-977.3	-3715.1	67.0	5.5	even	ok
	3	C 15 H 10 F 3 O	100.00	263.0689	-0.5	-2.0	93.9	9.5	even	ok