

# Mass Spectrum SmartFormula Report

## Analysis Info


Analysis Name E:\Data2\Kilian\CSA-1-38000001.d\CSA-1-20000001.d  
Method Tune\_low\_pos.m  
Sample Name naphtholKCy  
Comment

Acquisition Date 2018-06-12 16:39:00

Operator Carin Larsson  
Instrument / Ser# micrOTOF 125

## Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

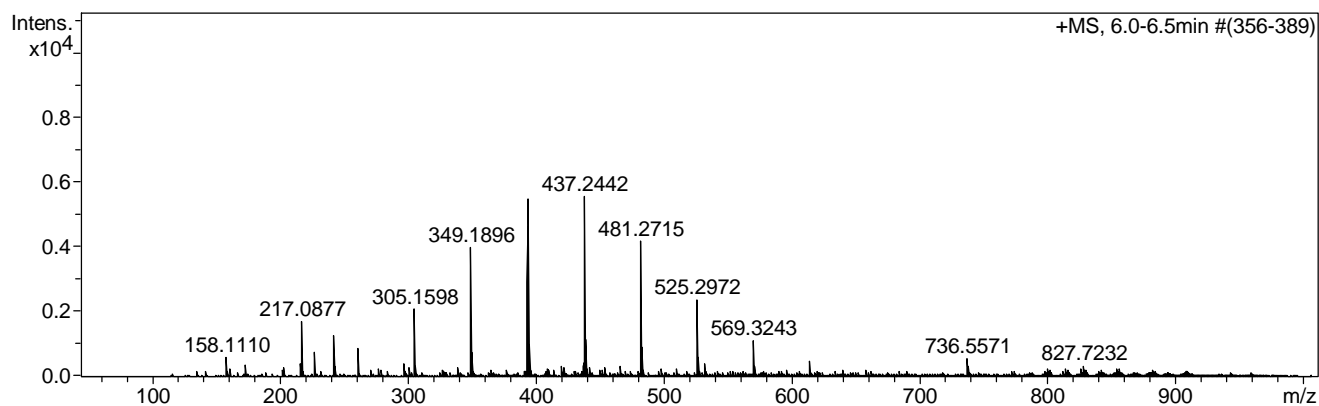

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e <sup>-</sup>	Conf	N-Rule
277.1211	1	C 17 H 18 Na O 2	100.00	277.1199	-1.2	-4.5	106.8	8.5	even		ok