

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\2pyKpOMe000001.d
Method Tune_low_pos.m
Sample Name 2PyKpOMe
Comment

Acquisition Date 2018-02-16 13:25:41

Operator Carin Larsson
Instrument / Ser# microTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

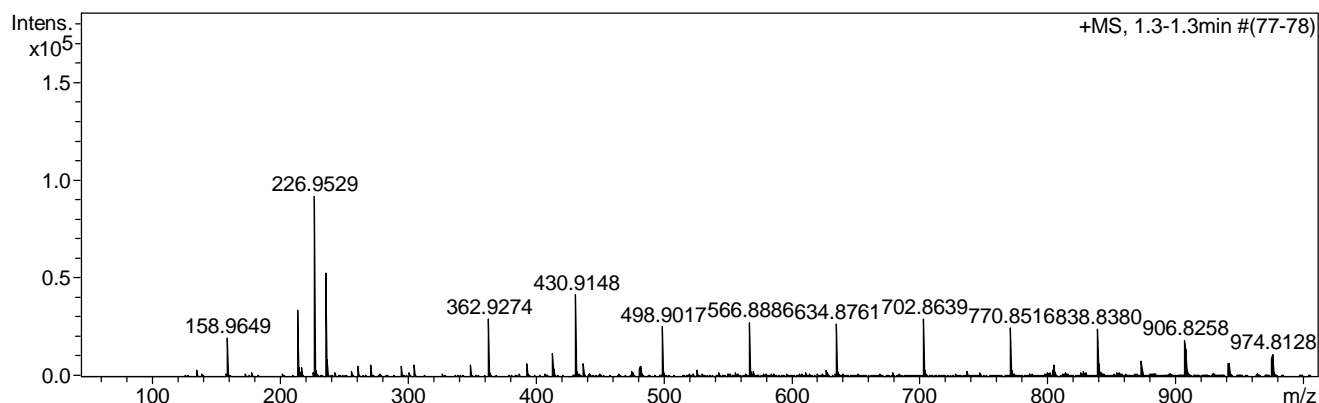

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻	Conf	N-Rule
214.0873	1	C 13 H 12 N O 2	100.00	214.0863	-1.0	-4.9	4.2	8.5	even		ok
236.0694	1	C 13 H 11 N Na O 2	100.00	236.0682	-1.2	-5.2	7.8	8.5	even		ok