

# Mass Spectrum SmartFormula Report

## Analysis Info


Analysis Name E:\Data2\Kilian\pClKpCF3000001.d  
Method Tune\_low\_pos.m  
Sample Name pClKpCF3  
Comment

Acquisition Date 2018-02-15 16:46:42

Operator Carin Larsson  
Instrument / Ser# microTOF 125

## Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

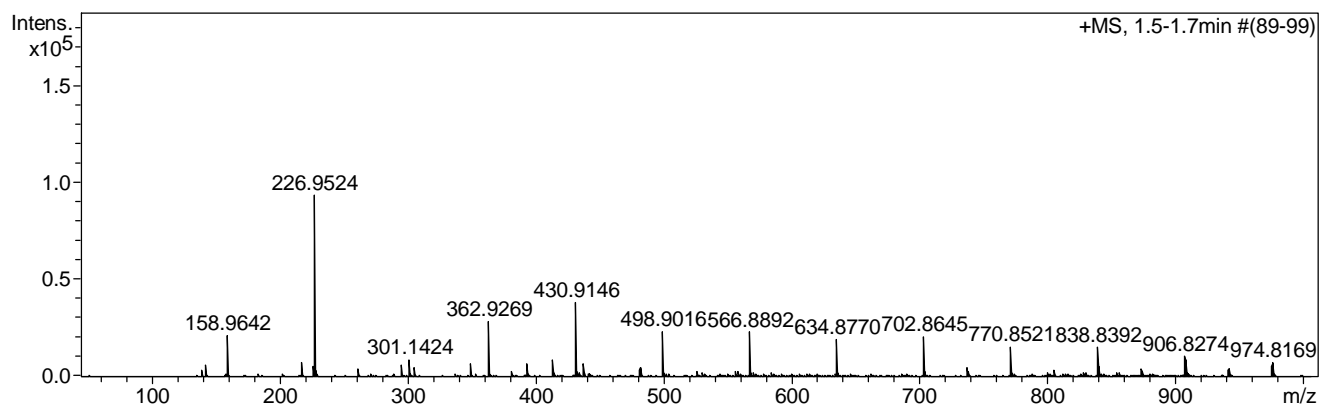

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdB	e <sup>-</sup> Conf	N-Rule
307.0103	1	C 14 H 8 Cl F 3 Na O	100.00	307.0108	0.5	1.7	172.6	8.5	even	ok
	2	C 7 H 8 Cl F 3 N 6 Na O	0.00	307.0292	19.0	61.8	195.6	4.5	even	ok
	3	C 10 H 8 Cl F 3 N 5 O	0.00	306.0364	-973.9	-3172.1	705.5	7.5	even	ok
	4	C 3 H 8 Cl F 3 N 11 O	0.00	306.0548	-955.4	-3112.0	725.3	3.5	even	ok