

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\CSA-1-49000001.d
Method Tune_low_pos.m
Sample Name the frog
Comment

Acquisition Date 2018-06-13 17:37:27

Operator Carin Larsson
Instrument / Ser# microTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

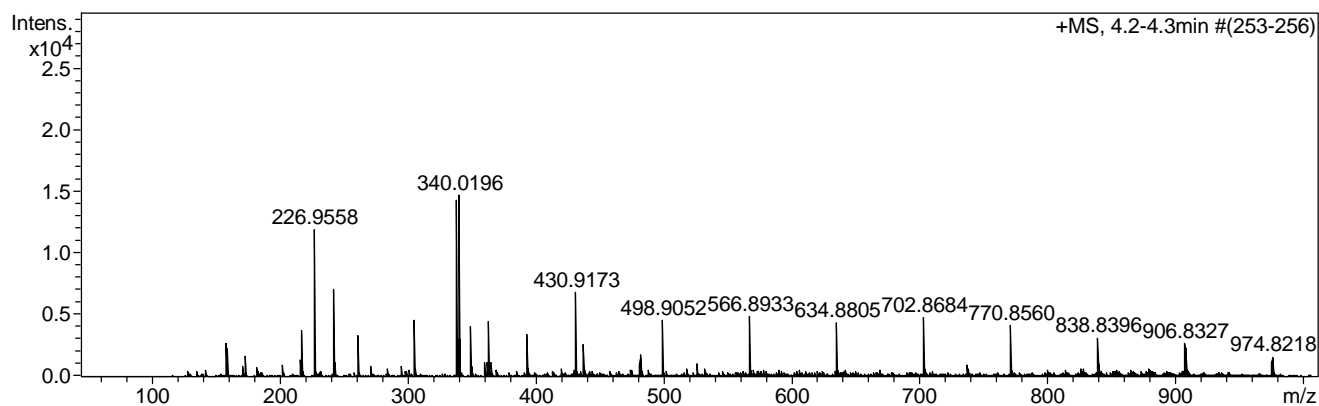

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻	Conf	N-Rule
231.0634	1	C 4 H 12 N 6 Na O 4	0.00	231.0812	17.8	77.2	38.1	1.5	even		ok
	2	C 11 H 12 Na O 4	100.00	231.0628	-0.6	-2.6	69.2	5.5	even		ok