

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\pOMeKpCF3000001.d
Method Tune_low_pos.m
Sample Name pOMeKpCF3
Comment

Acquisition Date 2018-02-15 16:54:52

Operator Carin Larsson
Instrument / Ser# microTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

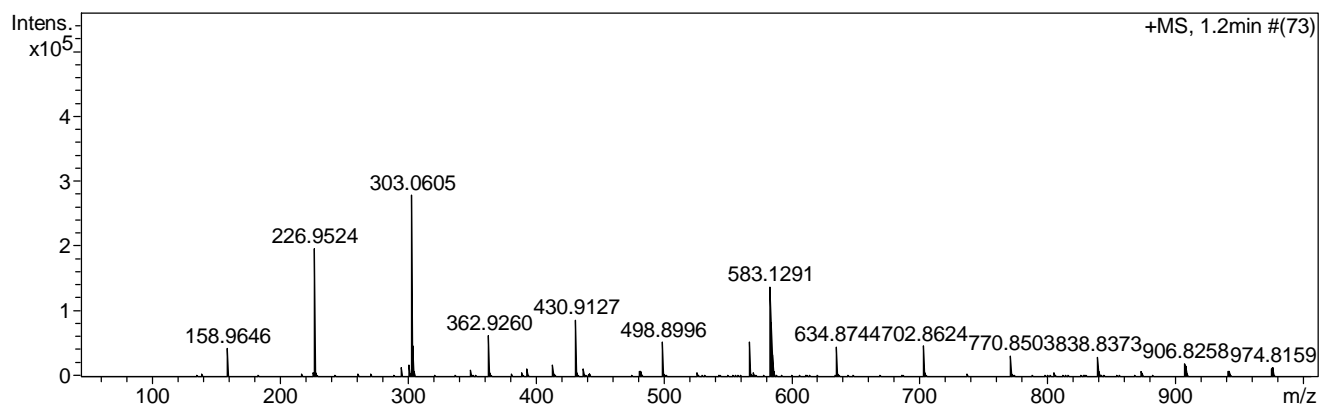

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSig ma	rdb	e ⁻ Conf	N-R ule
303.0605	1	C 15 H 11 F 3 Na O 2	100.00	303.0603	-0.2	-0.7	10.1	8.5	even	ok
	2	C 11 H 11 F 3 N 5 O 2	0.00	302.0859	-974.6	-3215.9	767.7	7.5	even	ok