

# Mass Spectrum SmartFormula Report

## Analysis Info


Analysis Name E:\Data2\BMM\_Alba\acc-218000001.d  
Method Tune\_low\_pos.m  
Sample Name acc-218  
Comment

Acquisition Date 2021-05-27 16:24:37

Operator Carin Larsson  
Instrument / Ser# micrOTOF 125

## Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4000 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

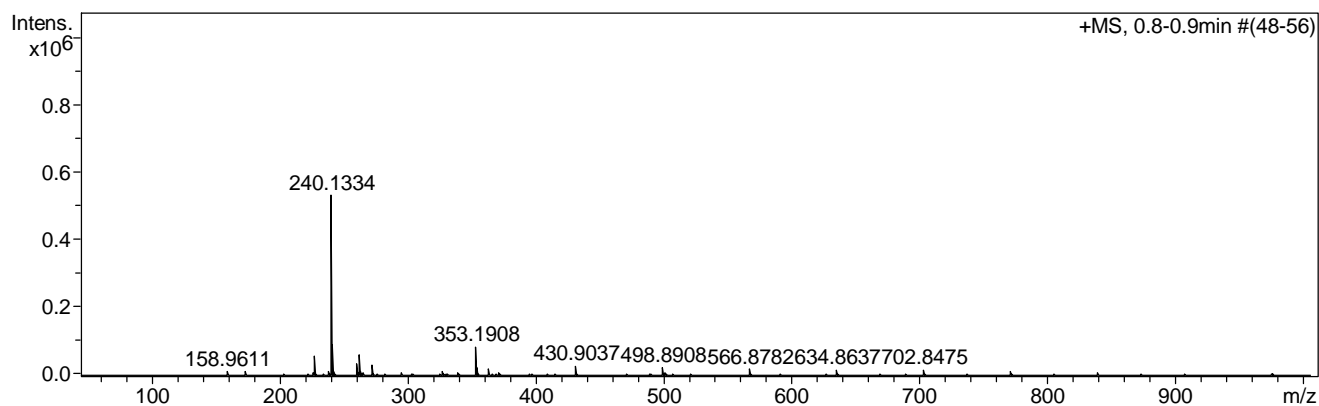

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e <sup>-</sup>	Conf	N-Rule
240.1334	1	C <sub>16</sub> H <sub>18</sub> N <sub>2</sub> O	100.00	240.1383	4.9	20.3	5.3	8.5	even		ok