

# Mass Spectrum SmartFormula Report

## Analysis Info


Analysis Name E:\Data2\Amparo\ASM-2034E000001.d  
Method Tune\_low\_pos.m  
Sample Name ASM-2034E  
Comment

Acquisition Date 2019-12-16 16:36:17

Operator Carin Larsson  
Instrument / Ser# micrOTOF 125

## Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4000 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Waste

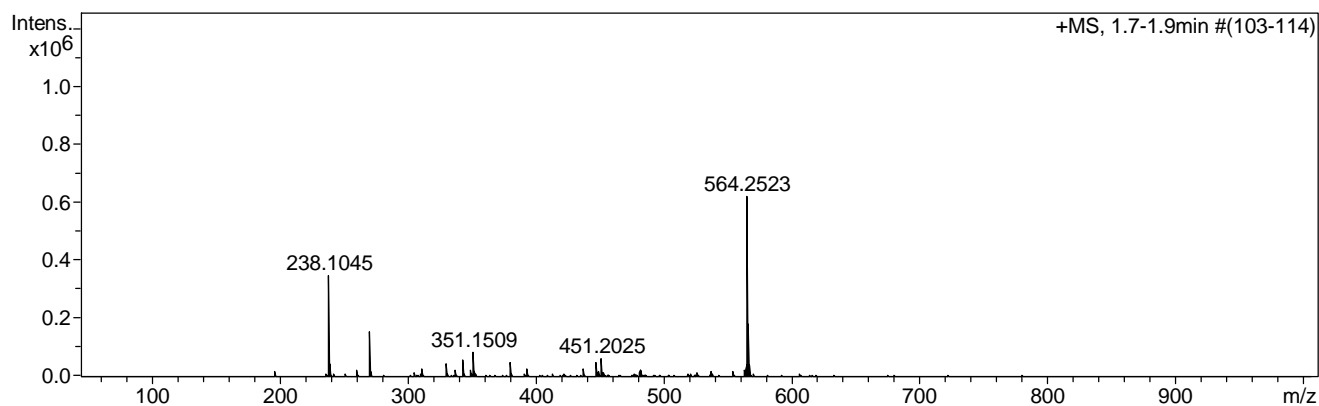

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e <sup>-</sup>	Conf	N-Rule
238.1045	1	C 10 H 17 N Na O 4	100.00	238.1050	0.5	2.0	12.0	2.5	even		ok