

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\BMM_Alba\ACCCARB-9000001.d
Method Tune_low_pos.m
Sample Name ACCCARB-9
Comment

Acquisition Date 2021-06-03 13:53:34

Operator Carin Larsson
Instrument / Ser# micrOTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4000 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

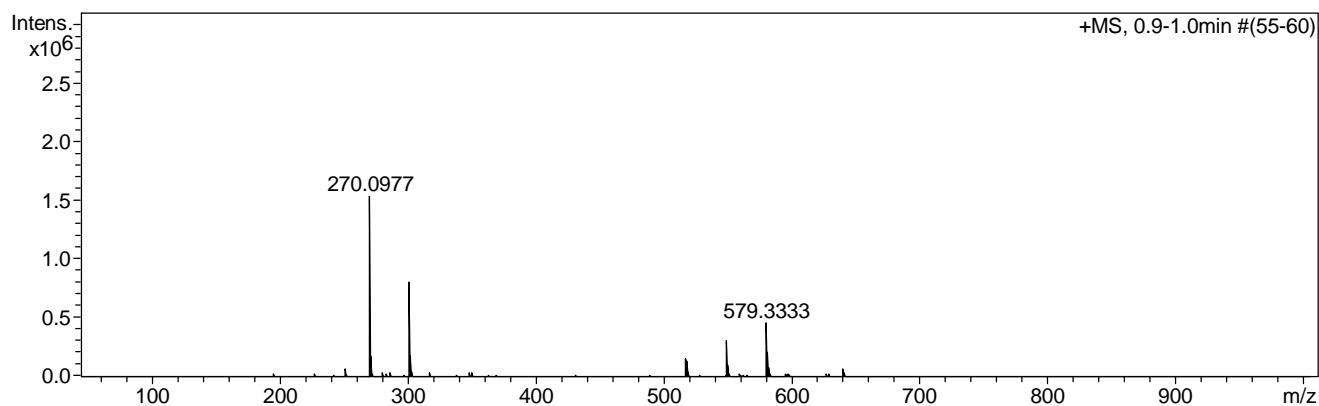

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻	Conf	N-Rule
270.0977	1	C 10 H 17 N Na O 6	100.00	270.0948	-2.9	-10.6	3.4	2.5	even		ok
	2	C 10 H 17 N Na O 6	100.00	270.0948	-2.9	-10.6	3.4	2.5	even		ok
	3	C 10 H 17 N Na O 6	100.00	270.0948	-2.9	-10.6	3.4	2.5	even		ok