

# Mass Spectrum SmartFormula Report

## Analysis Info


Analysis Name E:\Data2\BMM\_Alba\AC496p000001.d  
Method Tune\_low\_pos.m  
Sample Name AC496p  
Comment

Acquisition Date 2022-01-20 11:41:57

Operator Carin Larsson  
Instrument / Ser# microTOF 125

## Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4000 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

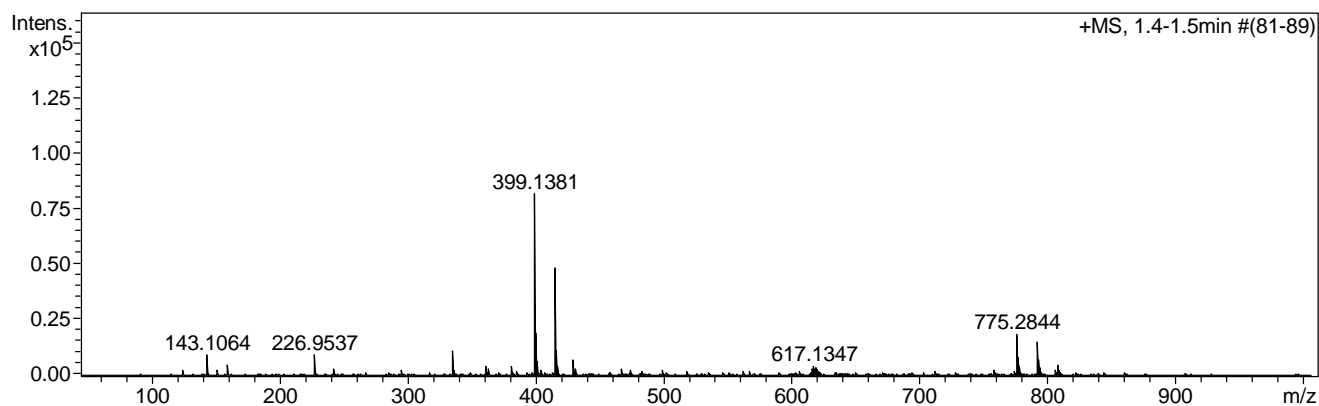

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSig ma	rdb	e <sup>-</sup> Conf	N-R ule
399.1381	1	C 19 H 24 N 2 Na O 4 S	100.00	399.1349	-3.2	-8.1	4.8	8.5	even	ok