

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\BMM_Alba\AC494p000001.d
Method Tune_low_pos.m
Sample Name AC494p
Comment

Acquisition Date 2022-01-20 10:58:33

Operator Carin Larsson
Instrument / Ser# micrOTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4000 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

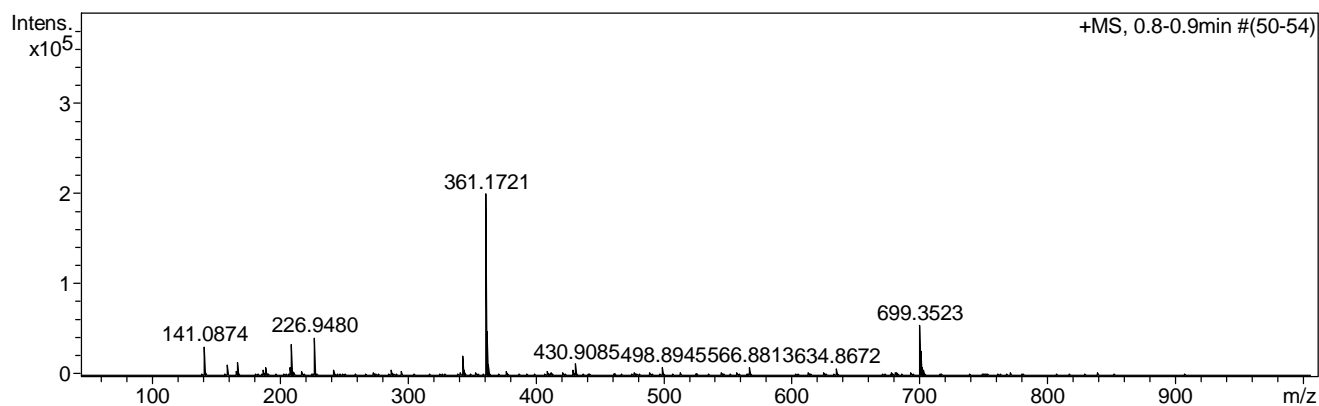

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻	Conf	N-Rule
361.1721	1	C 22 H 26 Na O 3	100.00	361.1774	5.4	14.8	6.1	9.5	even		ok