

# Mass Spectrum SmartFormula Report

## Analysis Info


Analysis Name E:\Data2\BMM\_Alba\526-ao000001.d  
Method Tune\_low\_pos.m  
Sample Name 526-ao  
Comment

Acquisition Date 2022-02-03 16:20:16

Operator Carin Larsson  
Instrument / Ser# microTOF 125

## Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4000 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

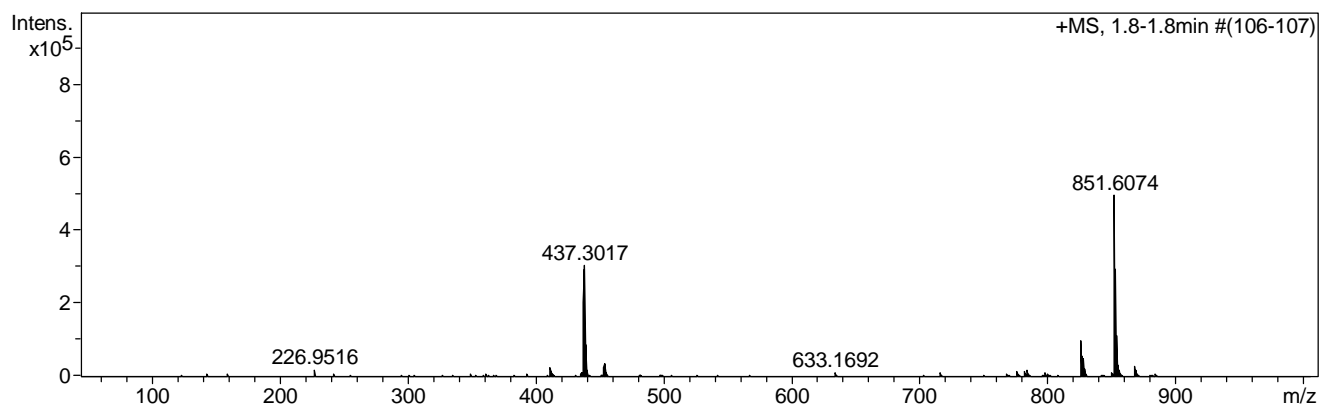

Formula	Meas. m/z	m/z	err [ppm]	Mean err [ppm]
C 27 H 42 Na O 3	437.3017	437.3026	2.0	1.9