

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\KC-5-PhSMePh-mgcl2000001.d
Method Tune_low_pos.m
Sample Name PhSMePh-mgcl2
Comment

Acquisition Date 2017-03-02 14:19:16

Operator Carin Larsson
Instrument / Ser# microTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

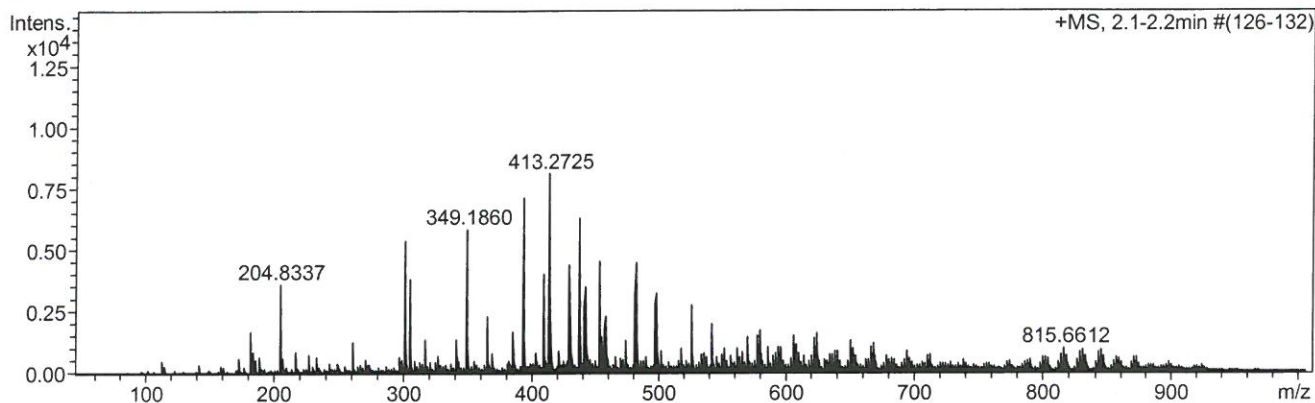

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻	Conf	N-Rule
201.0725	1	C 13 H 13 S	100.00	201.0732	0.7	3.6	441.5	7.5	even		ok

