

Modifier-Free Microfluidic Electrochemical Sensor for Heavy Metal Detection




TECHNISCHE
UNIVERSITÄT
DARMSTADT

Liu-Liu Shen, Gui-Rong Zhang, Wei Li, Markus Biesalski, Bastian J.M. Etzold

Heavy metals are hazard pollutants to the environment and impose severe risks to human health. Therefore, heavy metal detection is playing important role in environmental and clinical analysis. In this work, a simple, cost-effective and portable miniaturized electrochemical carbon-based sensor (μ CS) is designed and proved to be highly sensitive towards Cd^{2+} and Pb^{2+} detection in aqueous solution. The μ CS possess a novel 3D structure with working and reference electrodes directly facing each other but separated by the microfluidic paper channel. The electrodes in μ CS are inexpensive graphite foil without any additional surface modifier such as mercury or bismuth. It is found that impressive low detection limits of $1.2 \mu\text{g/L}$ for Cd^{2+} and $1.8 \mu\text{g/L}$ for Pb^{2+} can be achieved on the μ CS. The μ CS also exhibits stable sensing performance up to 10 repetitive measurements, demonstrating the robustness of a sensing device for heavy metal detections. We believe that a proper design in the device configuration can completely eliminate the necessity to modify the working electrode by using additional surface modifier, which could provide new ideas for portable electroanalytical/sensing systems.

Experimental Section

Device fabrication:

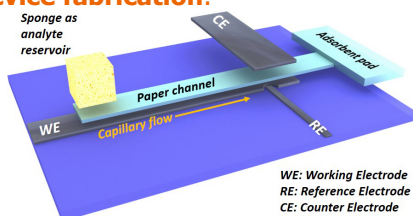


WE, CE & RE:
graphite foil

Paper channel:
filter paper,
pore size $15 \mu\text{m}$


Electrochemical measurements

1. Metal deposition; 2. Square wave voltammetry

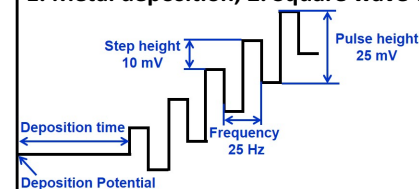


Electrolyte:
0.1 M acetate
buffer, pH=4.6


Individual detection of Cd^{2+} and Pb^{2+}

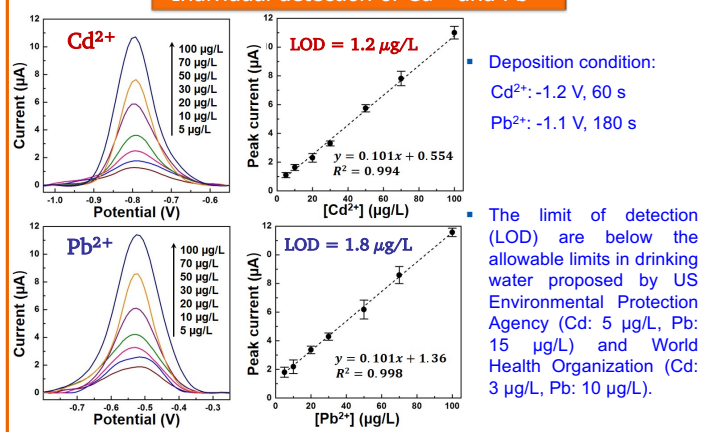


Simultaneous detection of Cd^{2+} and Pb^{2+}

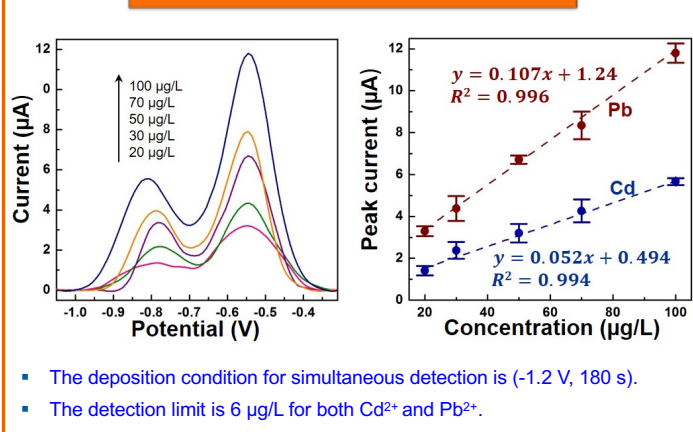

Stability and reproducibility of the μ CS

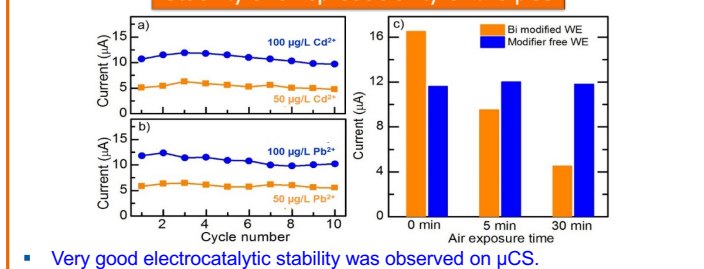

Structure analysis of the graphite foil

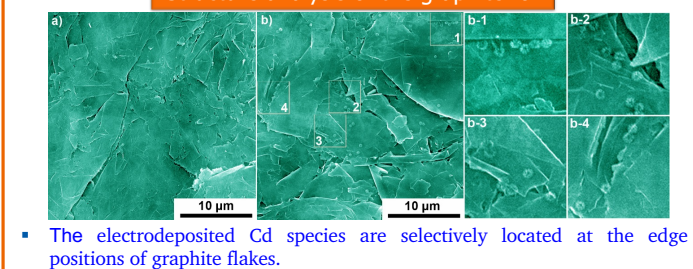

Conclusions:

- A modifier-free, low cost, reusable, electrochemical microfluidic carbon-based sensor was developed for heavy metal detection.
- High sensitivity and low detection limit at short detection time are obtained on the sensor during individual detection for Cd^{2+} and Pb^{2+} .
- The high sensitivity may originate from the combined microfluidic configuration and novel 3D electrode layout, which may provide some new ideas for other portable electroanalytical/sensing systems.

Correspondence:

Prof. Bastian J.M. Etzold (etzold@tc1.tu-darmstadt.de)
Ernst-Berl-Institut für Technische und Makromolekulare Chemie
Technische Universität Darmstadt
64287 Darmstadt

This project has received funding from the European Research Council (ERC) under the European Union's Horizon 2020 research and innovation programme (grant agreement n° 681719)

References:

- P. Lodeiro, J. Barriada, R. Herrero, M.S. De Vicente, *Environ. Pollut.* 2006, 142, 264.
- P. Apostoli, *J. Chromatogr. B* 2002, 778, 63.
- Table of regulated drinking water contaminants. <https://www.epa.gov/>
- Guidelines for drinking water quality, 4th ed. World Health Organization: Geneva, 2011.
- L. Shen, G. Zhang, W. Li, M. Biesalski, B. J. M. Etzold, *ACS Omega* in submission.