

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Rodrigo_AM\ROD-3-091000001.d
Method Tune_low_pos.m
Sample Name ROD-3-091
Comment Acetonitrile

Acquisition Date 2018-05-07 12:34:25

Operator Carin Larsson
Instrument / Ser# micrOTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

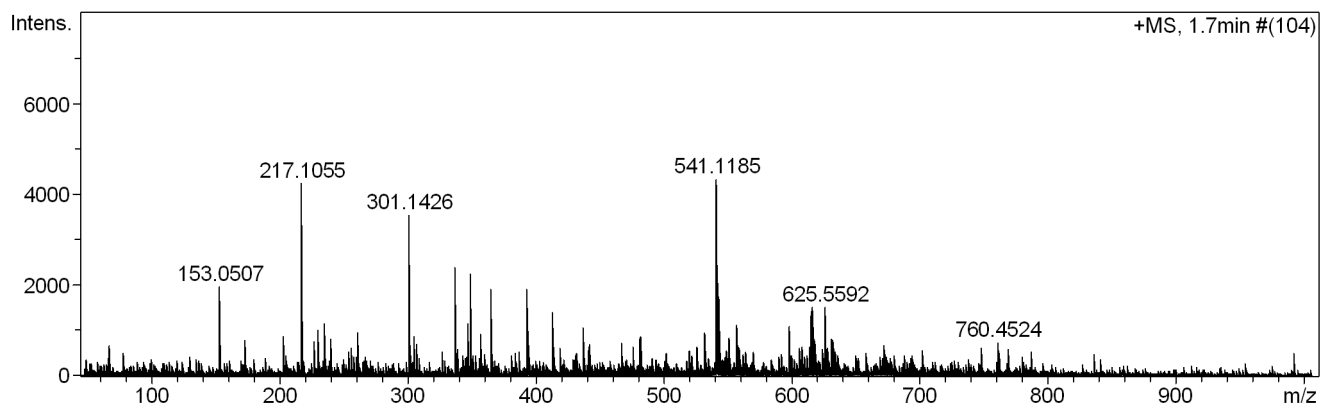

Formula	Meas. m/z	m/z	err [ppm]	Mean err [ppm]
C 10 H 12 F 2 N 6 Na O Se	373.2276	373.0098	-583.5	
C 15 H 12 F 2 Na O Se	348.9910	348.9914	1.1	0.7