

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Rodrigo_AM\ROD-1-068000001.d
Method Tune_low_pos.m
Sample Name ROD-1-068
Comment MeOH, lowpos

Acquisition Date 2018-01-12 18:09:30


Operator Carin Larsson
Instrument / Ser# micrOTOF 125

Acquisition Parameter


Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

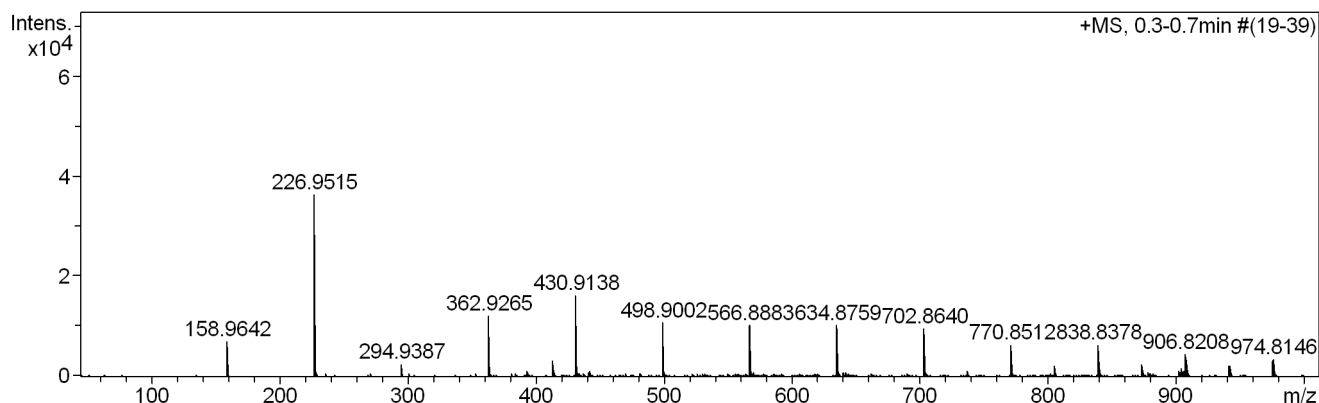

Formula	Meas. m/z	m/z	err [ppm]	Mean err [ppm]
C 14 H 17 F 2 O	239.1235	239.1242	3.0	3.0

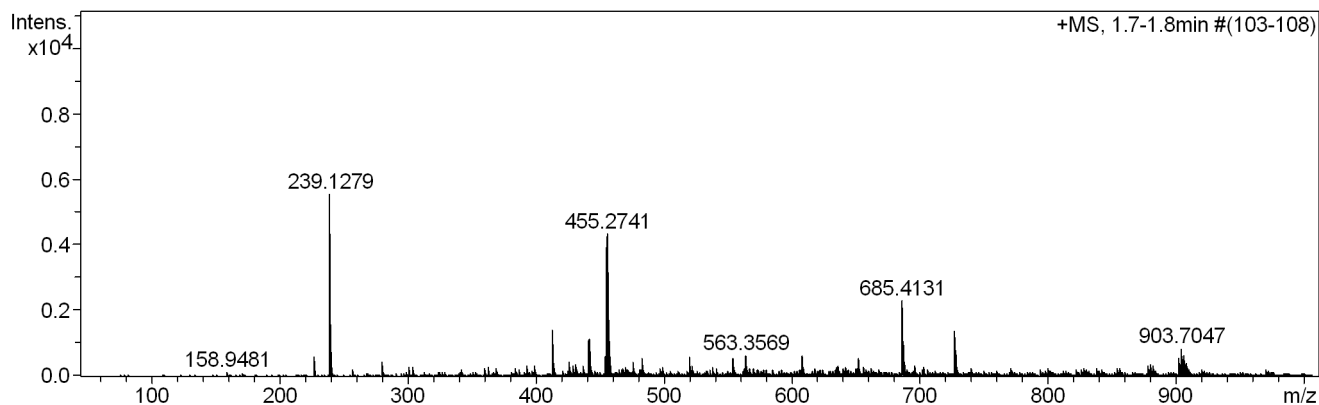

Formula	Meas. m/z	m/z	err [ppm]	Mean err [ppm]
C 14 H 17 F 2 O	239.1279	239.1242	-15.3	-15.2

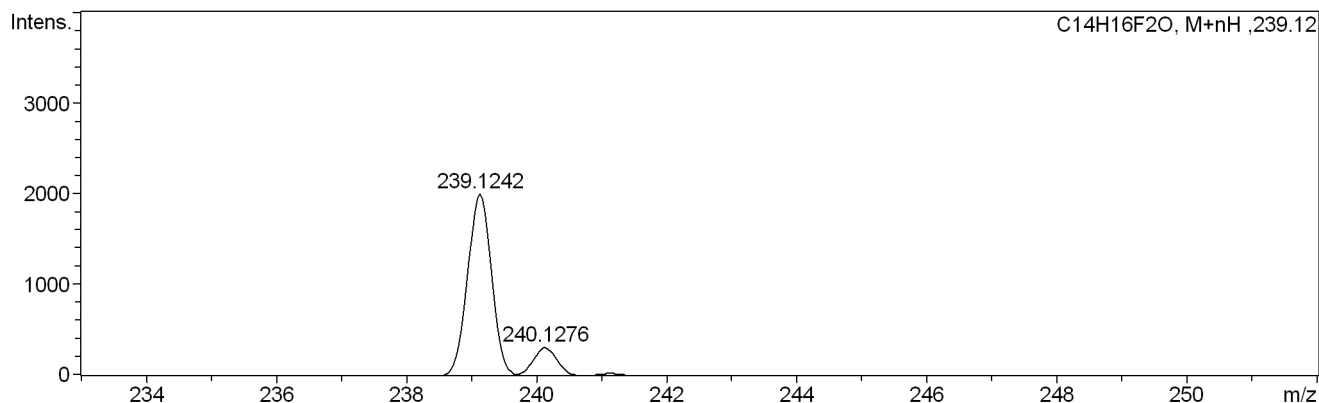

Formula	Meas. m/z	m/z	err [ppm]	Mean err [ppm]
---------	-----------	-----	-----------	----------------