

Mass Spectrum SmartFormula Report

Analysis Info


Analysis Name E:\Data2\Kilian\KC-5-FcSMetBu.d
Method Tune_low_pos.m
Sample Name FcSMetBu
Comment

Acquisition Date 2016-12-09 18:40:02

Operator Carin Larsson
Instrument / Ser# microTOF 125

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Not active			Set Dry Heater	180 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	4.0 l/min
Scan End	1000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Source

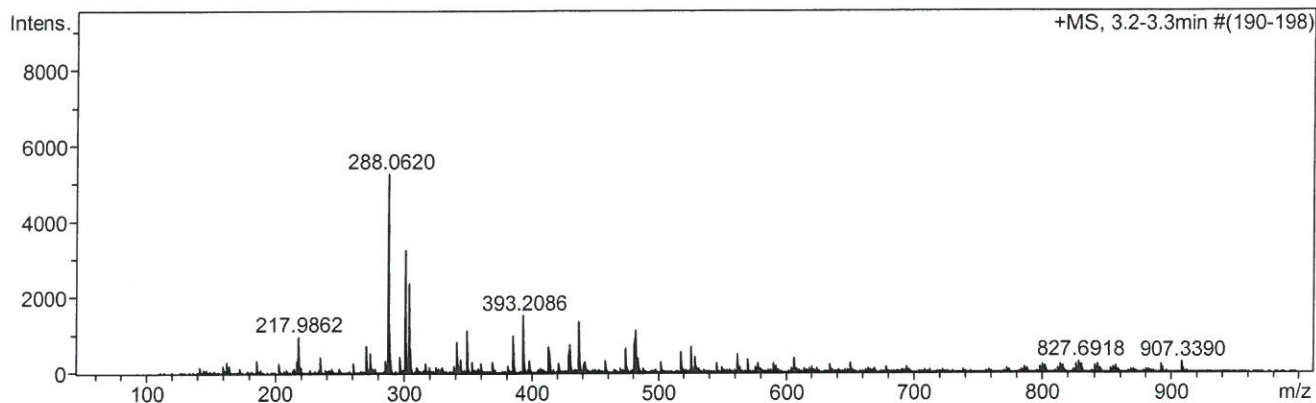

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e ⁻	Conf	N-Rule
288.0620	1	C 15 H 20 Fe S	100.00	288.0630	0.9	3.2	580.8	6.0	odd		ok

