


Sample Name: U1553A 18H6

=====

Acq. Operator : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : NGA-2 Location : 1 (F)
Injection Date : 1/15/2020 11:00:48 PM
Inj Volume : Manual ly
Method : C:\Chem32\2\Methods\378T_NGA2_TCD0FF.M
Last changed : 1/15/2020 5:13:03 PM by SYSTEM
(modified after loading)
Method Info : manual headspace injections
Sample Info : cyl 10751261

Sample-related custom fields:

Name	Value
------	-------

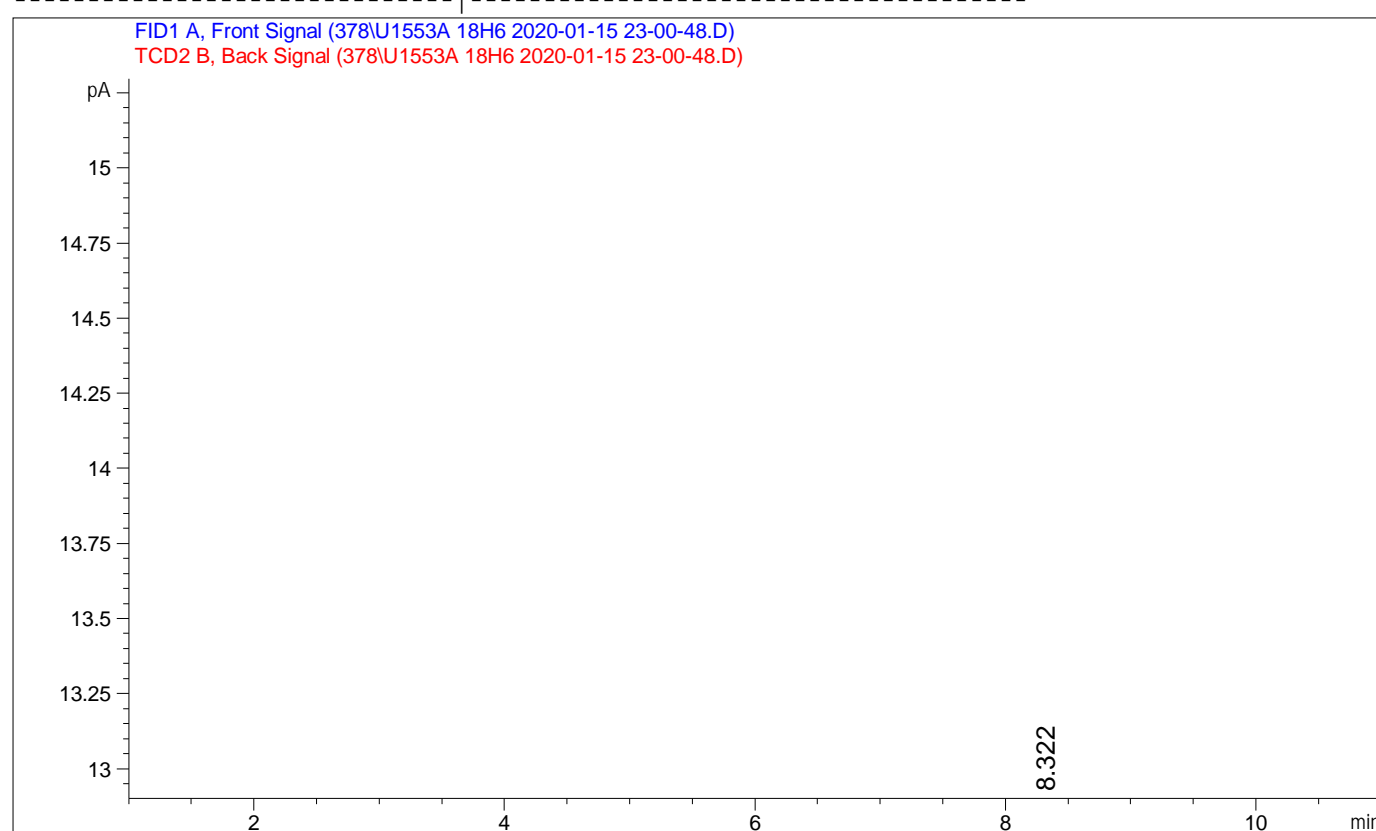

=====

External Standard Report

=====

Sorted By : Signal
Calib. Data Modified : 1/15/2020 5:12:59 PM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ppm]	Grp	Name
1.610	-	-	-	-	-	methane
1.990	-	-	-	-	-	ethane
2.714	-	-	-	-	-	ethene
4.024	-	-	-	-	-	propane
6.340	-	-	-	-	-	propene
6.736	-	-	-	-	-	i so-butane
6.967	-	-	-	-	-	n-butane
8.544	-	-	-	-	-	i so-pentane
8.697	-	-	-	-	-	n-pentane
9.902	-	-	-	-	-	i so-hexane
10.068	-	-	-	-	-	n-hexane

Totals : 0.00000

Signal 2: TCD2 B, Back Signal

RetTime [min]	Type	Area [25 μ V*s]	Amt/Area	Amount [ppm]	Grp	Name
4.598	-	-	-	-	0	
5.414	-	-	-	-	N	

Totals : 0.00000

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Time reference compound(s) not found

```
=====
Summed Peaks Report
=====
```

Signal 1: FID1 A, Front Signal
Empty table.

Signal 2: TCD2 B, Back Signal
Empty table.

```
=====
Final Summed Peaks Report
=====
```

Signal 1: FID1 A, Front Signal

Sample Name: U1553A 18H6

Name	Total Area [25 μ V*s]	Amount [ppm]
methane	0.00000	0.0000
ethane	0.00000	0.0000
ethene	0.00000	0.0000
propane	0.00000	0.0000
propene	0.00000	0.0000
i so-butane	0.00000	0.0000
n-butane	0.00000	0.0000
i so-pentane	0.00000	0.0000
n-pentane	0.00000	0.0000
i so-hexane	0.00000	0.0000
n-hexane	0.00000	0.0000

Totals : 0.0000

Signal 2: TCD2 B, Back Signal

Name	Total Area [25 μ V*s]	Amount [ppm]
O	0.00000	0.0000
N	0.00000	0.0000

Totals : 0.0000

=====
Area Percent Report
=====

Sorted By : Signal
 Calib. Data Modified : 1/15/2020 5:12:59 PM
 Multiplier : 1.0000
 Dilution : 1.0000
 Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.610	+	0.0000	0.00000	0.00000	methane
2	1.990	+	0.0000	0.00000	0.00000	ethane
3	2.714	+	0.0000	0.00000	0.00000	ethene
4	4.024	+	0.0000	0.00000	0.00000	propane
5	6.340	+	0.0000	0.00000	0.00000	propene
6	6.736	+	0.0000	0.00000	0.00000	i so-butane
7	6.967	+	0.0000	0.00000	0.00000	n-butane
8	8.544	+	0.0000	0.00000	0.00000	i so-pentane
9	8.697	+	0.0000	0.00000	0.00000	n-pentane
10	9.902	+	0.0000	0.00000	0.00000	i so-hexane
11	10.068	+	0.0000	0.00000	0.00000	n-hexane

Totals : 0.00000 0.0000

Signal 2: TCD2 B, Back Signal

Peak #	RetTime [min]	Type	Width [min]	Area [25 µV*s]	Area %	Name
1	4.598		0.0000	0.00000	0.00000	O
2	5.414		0.0000	0.00000	0.00000	N

Totals : 0.00000 0.0000

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Time reference compound(s) not found

=====

=====

Summed Peaks Report

=====

Signal 1: FID1 A, Front Signal

Empty table.

Signal 2: TCD2 B, Back Signal

Empty table.

=====

Final Summed Peaks Report

=====

Signal 1: FID1 A, Front Signal

Name	Total Area [25 µV*s]	Area %
methane	0.00000	0.0000
ethane	0.00000	0.0000
ethene	0.00000	0.0000
propane	0.00000	0.0000
propene	0.00000	0.0000
i so-butane	0.00000	0.0000
n-butane	0.00000	0.0000
i so-pentane	0.00000	0.0000
n-pentane	0.00000	0.0000
i so-hexane	0.00000	0.0000
n-hexane	0.00000	0.0000

Totals : 0.0000

Signal 2: TCD2 B, Back Signal

Name	Total Area [25 µV*s]	Area %
O	0.00000	0.0000
N	0.00000	0.0000

Name	Total Area [25 μ V*s]	Area %
----- ----- -----		
Totals :		0.0000

Compound-related custom fields:

*** End of Report ***