

Sample Name: 396-U1570A-10R-CC-HS

=====


Acq. Operator : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : NGA-2 Location : - (F)
Injection Date : 8/31/2021 2:23:51 PM
Inj Volume : Manual ly

Method : C:\CHEM32\2\METHODS\396_NGA2.M
Last changed : 8/29/2021 8:30:11 PM by SYSTEM
Method Info : manual headspace injections

Sample Info : CYL11124781

Sample-related custom fields:

Name	Value
------	-------

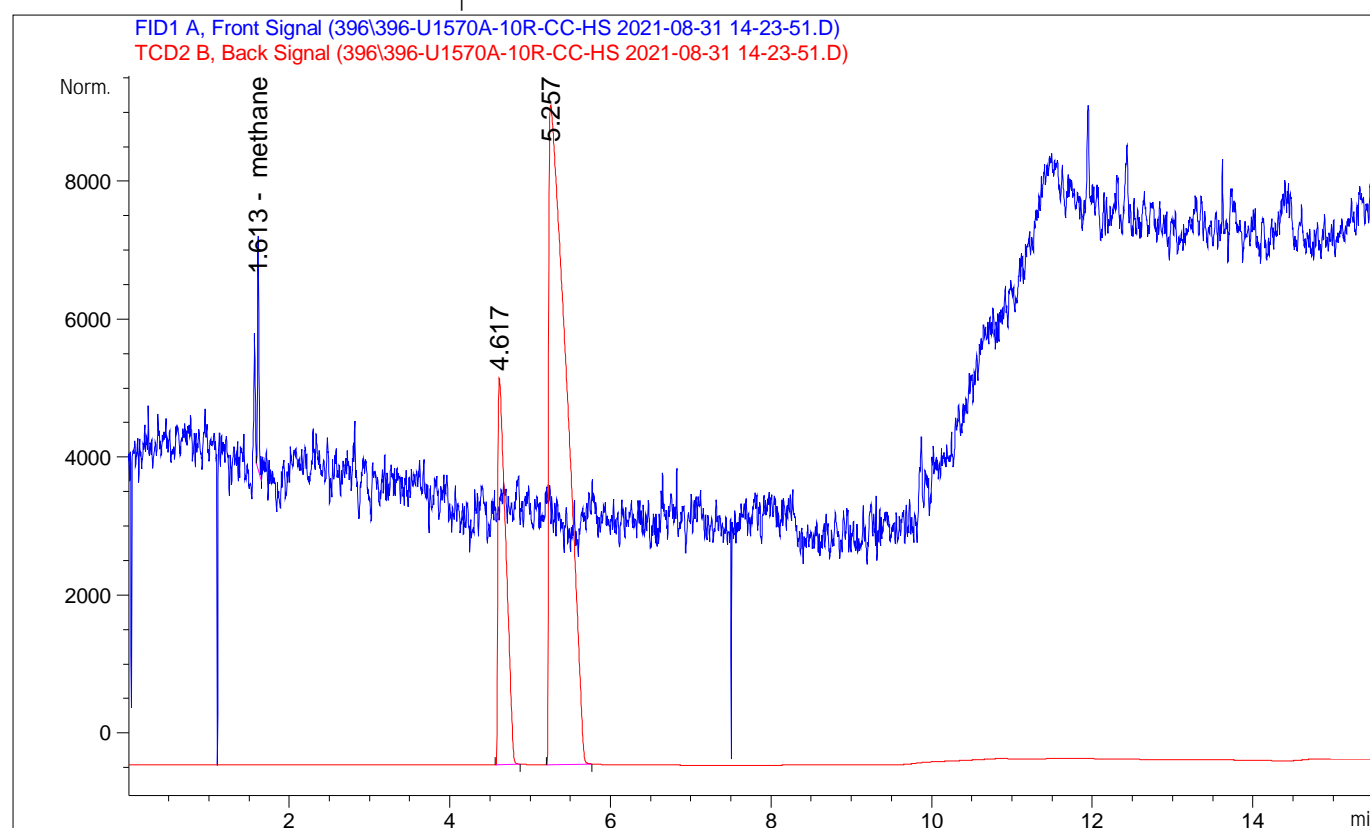

=====

External Standard Report

=====

Sorted By : Signal
Calib. Data Modified : 8/29/2021 4:44:17 PM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ppm]	Grp	Name
1.613	BB	1.14740e-1	10.39263	1.19245		methane
1.988		-	-	-		ethane
2.712		-	-	-		ethene
3.999		-	-	-		propane
6.334		-	-	-		propene
6.700		-	-	-		i so-butane
6.932		-	-	-		n-butane
8.505		-	-	-		i so-pentane
8.657		-	-	-		n-pentane
9.855		-	-	-		i so-hexane
10.020		-	-	-		n-hexane

Totals : 1.19245

Signal 2: TCD2 B, Back Signal

RetTime [min]	Type	Area [25 μ V*s]	Amt/Area	Amount [ppm]	Grp	Name
10.540		-	-	-		carbon dioxide

Totals : 0.00000

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

Summed Peaks Report

Signal 1: FID1 A, Front Signal
Empty table.

Signal 2: TCD2 B, Back Signal
Empty table.

Final Summed Peaks Report

Signal 1: FID1 A, Front Signal

Name	Total Area [25 μ V*s]	Amount [ppm]
methane	1.14740e-1	1.1924
ethane	0.00000	0.0000
ethene	0.00000	0.0000

Name	Total Area [25 μ V*s]	Amount [ppm]
----- ----- -----		
propane	0.00000	0.0000
propene	0.00000	0.0000
i so-butane	0.00000	0.0000
n-butane	0.00000	0.0000
i so-pentane	0.00000	0.0000
n-pentane	0.00000	0.0000
i so-hexane	0.00000	0.0000
n-hexane	0.00000	0.0000

Totals : 1.1924

Signal 2: TCD2 B, Back Signal

Name	Total Area [25 μ V*s]	Amount [ppm]
----- ----- -----		
carbon di oxide	0.00000	0.0000

Totals : 0.0000

Compound-related custom fields:

*** End of Report ***