

Sample Name: 396-U1566A-2R-1-HS


```
=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : NGA-2                      Location :      - (F)
Injection Date  : 8/16/2021 7:12:23 AM
                                           Inj Volume : Manual ly

Method          : C:\CHEM32\2\METHODS\396_NGA2.M
Last changed    : 8/15/2021 6:26:54 PM by SYSTEM
                  (modified after loading)
Method Info     : manual headspace injections

Sample Info     : CYL11056421
=====
```

Sample-related custom fields:

Name	Value
------	-------

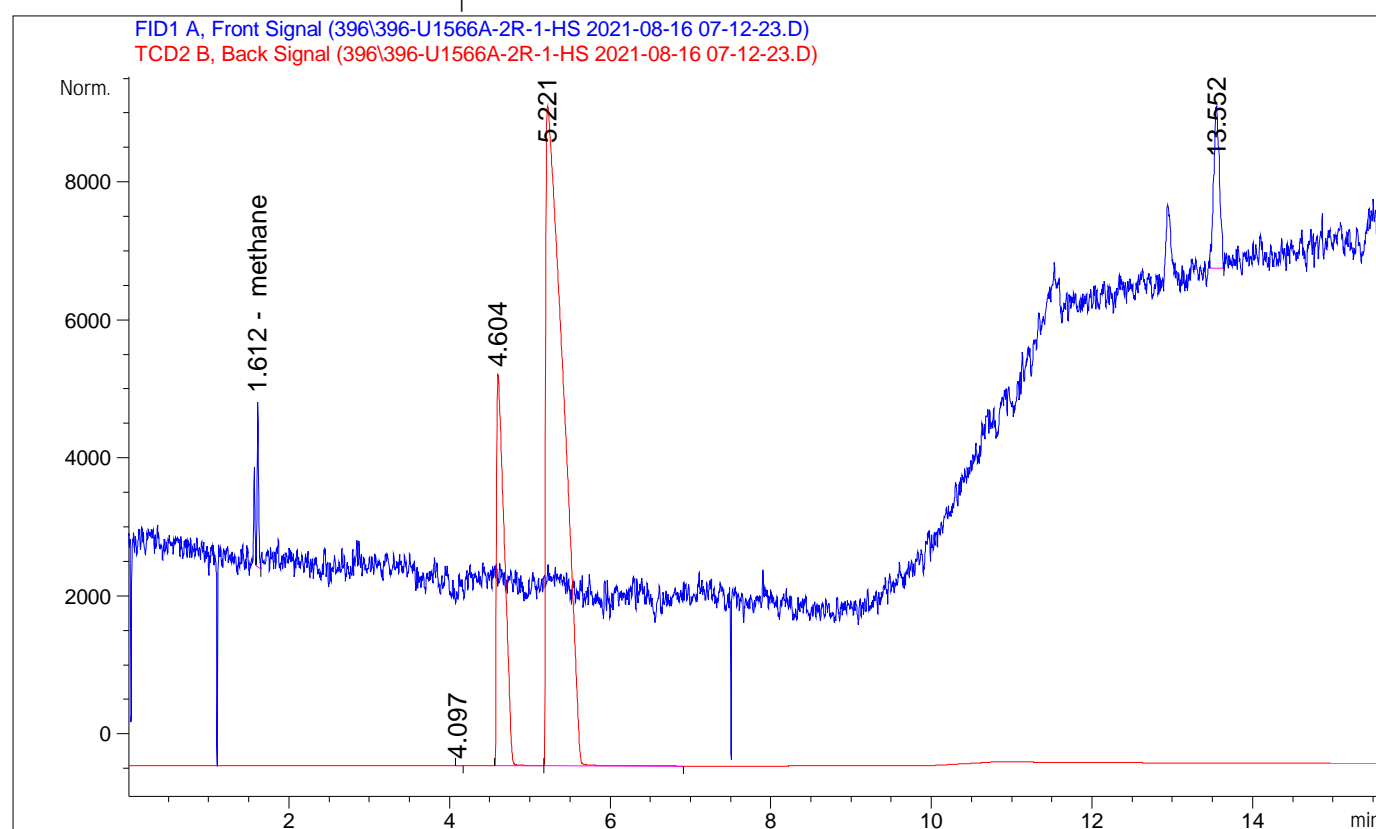

```
=====
External Standard Report
=====
```

```
Sorted By      :      Signal
Calib. Data Modified :      8/11/2021 10:16:43 PM
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ppm]	Grp	Name
1.612	VB	1.17882e-1	8.18872	9.65299e-1		methane
1.990		-	-	-		ethane
2.731		-	-	-		ethene
3.989		-	-	-		propane
6.355		-	-	-		propene
6.717		-	-	-		i so-butane
6.947		-	-	-		n-butane
8.519		-	-	-		i so-pentane
8.672		-	-	-		n-pentane
9.871		-	-	-		i so-hexane
10.036		-	-	-		n-hexane

Totals : 9.65299e-1

Signal 2: TCD2 B, Back Signal

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

Summed Peaks Report

Signal 1: FID1 A, Front Signal

Empty table.

Signal 2: TCD2 B, Back Signal

Empty table.

Final Summed Peaks Report

Signal 1: FID1 A, Front Signal

Name	Total Area [25 μ V*s]	Amount [ppm]
methane	1.17882e-1	0.9653
ethane	0.00000	0.0000
ethene	0.00000	0.0000
propane	0.00000	0.0000
propene	0.00000	0.0000
i so-butane	0.00000	0.0000
n-butane	0.00000	0.0000
i so-pentane	0.00000	0.0000

Name	Total Area [25 μ V*s]	Amount [ppm]
----- ----- -----		
n-pentane	0.00000	0.0000
i so-hexane	0.00000	0.0000
n-hexane	0.00000	0.0000

Totals : 9.6530e-1

Signal 2: TCD2 B, Back Signal

Compound-related custom fields:

*** End of Report ***