


=====

Acq. Operator	: SYSTEM	
Sample Operator	: SYSTEM	
Acq. Instrument	: NGA-2	Location : - (F)
Injection Date	: 8/29/2021 2:25:32 AM	
		Inj Volume : Manual ly
Method	: C:\CHEM32\2\METHODS\396_NGA2.M	
Last changed	: 8/24/2021 10:19:38 PM by SYSTEM	
	(modified after loading)	
Method Info	: manual headspace injections	
Sample Info	: CYL11117211	

Sample-related custom fields:

Name	Value
------	-------

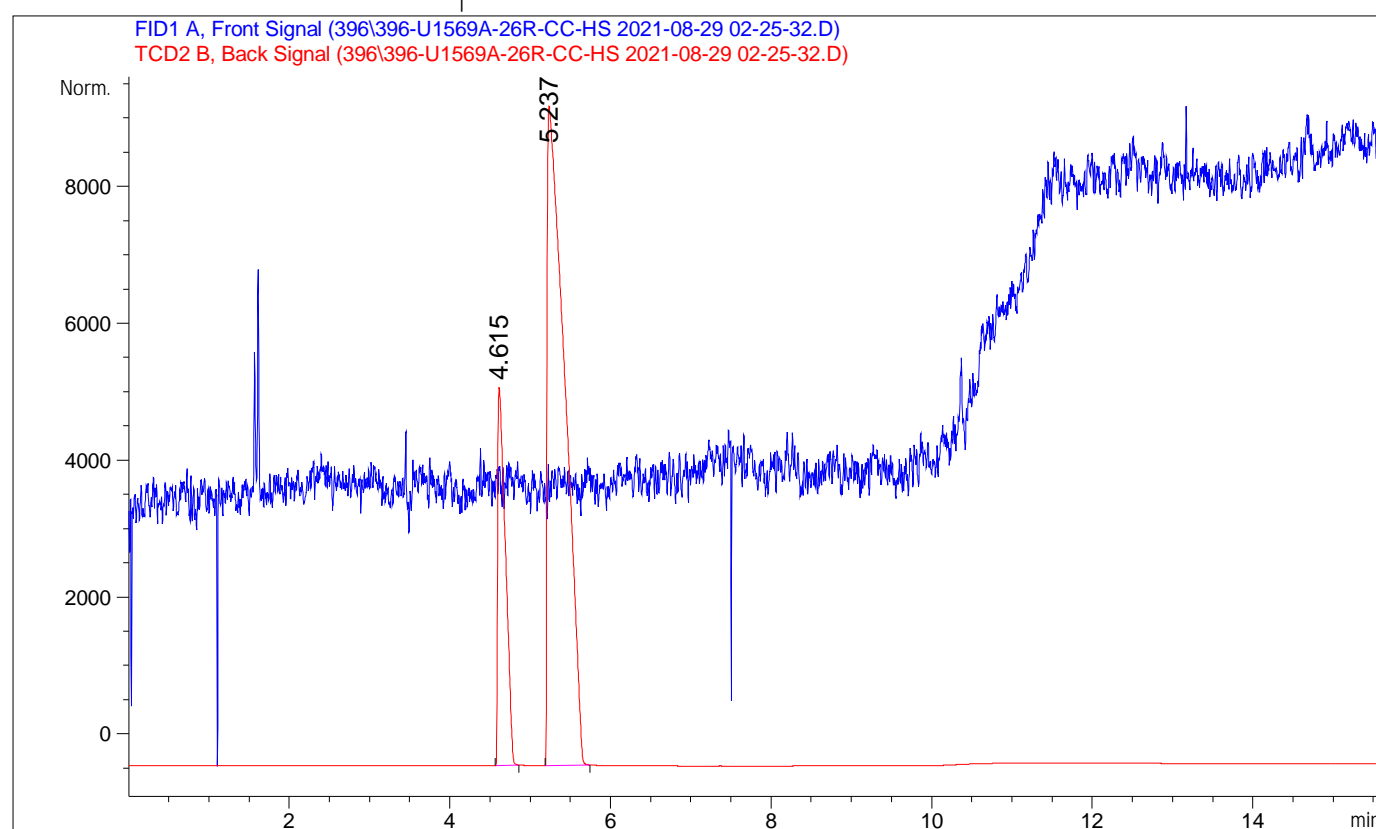

External Standard Report

=====

Sorted By	: Signal
Calib. Data Modified	: 8/21/2021 2:01:44 PM
Multiplier	: 1.0000
Dilution	: 1.0000

Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ppm]	Grp	Name
1.613		-	-	-		methane
1.988		-	-	-		ethane
2.712		-	-	-		ethene
3.999		-	-	-		propane
6.334		-	-	-		propene
6.700		-	-	-		i so-butane
6.932		-	-	-		n-butane
8.505		-	-	-		i so-pentane
8.657		-	-	-		n-pentane
9.855		-	-	-		i so-hexane
10.020		-	-	-		n-hexane

Totals : 0.00000

Signal 2: TCD2 B, Back Signal

RetTime [min]	Type	Area [25 µV*s]	Amt/Area	Amount [ppm]	Grp	Name
10.540		-	-	-		carbon di oxide

Totals : 0.00000

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====

=====

Summed Peaks Report

=====

Signal 1: FID1 A, Front Signal

Empty table.

Signal 2: TCD2 B, Back Signal

Empty table.

=====

Final Summed Peaks Report

=====

Signal 1: FID1 A, Front Signal

Name	Total Area [25 $\mu$ V*s]	Amount [ppm]
----- ----- -----		
methane	0.00000	0.0000
ethane	0.00000	0.0000
ethene	0.00000	0.0000
propane	0.00000	0.0000
propene	0.00000	0.0000
i so-butane	0.00000	0.0000
n-butane	0.00000	0.0000
i so-pentane	0.00000	0.0000
n-pentane	0.00000	0.0000
i so-hexane	0.00000	0.0000
n-hexane	0.00000	0.0000

Totals : 0.0000

Signal 2: TCD2 B, Back Signal

Name	Total Area [25 $\mu$ V*s]	Amount [ppm]
----- ----- -----		
carbon di oxide	0.00000	0.0000

Totals : 0.0000

=====  
Area Percent Report  
=====

Sorted By : Signal  
Calib. Data Modified : 8/21/2021 2:01:44 PM  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
----	-----	-----	-----	-----	-----	-----
1	1.613		0.0000	0.00000	0.00000	methane
2	1.988		0.0000	0.00000	0.00000	ethane
3	2.712		0.0000	0.00000	0.00000	ethene
4	3.999		0.0000	0.00000	0.00000	propane
5	6.334		0.0000	0.00000	0.00000	propene
6	6.700		0.0000	0.00000	0.00000	i so-butane
7	6.932		0.0000	0.00000	0.00000	n-butane
8	8.505		0.0000	0.00000	0.00000	i so-pentane
9	8.657		0.0000	0.00000	0.00000	n-pentane
10	9.855		0.0000	0.00000	0.00000	i so-hexane
11	10.020		0.0000	0.00000	0.00000	n-hexane

Totals : 0.00000 0.0000

Signal 2: TCD2 B, Back Signal

Peak #	RetTime [min]	Type	Width [min]	Area [25 µV*s]	Area %	Name
1	10.540		0.0000	0.00000	0.00000	carbon di oxide

Totals : 0.00000 0.0000

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====

=====

Summed Peaks Report

=====

Signal 1: FID1 A, Front Signal

Empty table.

Signal 2: TCD2 B, Back Signal

Empty table.

=====

Final Summed Peaks Report

=====

Signal 1: FID1 A, Front Signal

Name	Total Area [25 µV*s]	Area %
methane	0.00000	0.0000
ethane	0.00000	0.0000
ethene	0.00000	0.0000
propane	0.00000	0.0000
propene	0.00000	0.0000
i so-butane	0.00000	0.0000
n-butane	0.00000	0.0000
i so-pentane	0.00000	0.0000
n-pentane	0.00000	0.0000
i so-hexane	0.00000	0.0000
n-hexane	0.00000	0.0000

Totals : 0.0000

Signal 2: TCD2 B, Back Signal

Name	Total Area [25 µV*s]	Area %
carbon di oxide	0.00000	0.0000

Totals : 0.0000

Compound-related custom fields:

\*\*\* End of Report \*\*\*