


```
=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : NGA-2                      Location :      - (F)
Injection Date  : 8/28/2021 7:21:36 PM
                                           Inj Volume : Manual ly

Method          : C:\CHEM32\2\METHODS\396_NGA2.M
Last changed    : 8/24/2021 10:19:38 PM by SYSTEM
                  (modified after loading)
Method Info     : manual headspace injections

Sample Info     : CYL11115761
=====
```

Sample-related custom fields:

Name	Value
------	-------

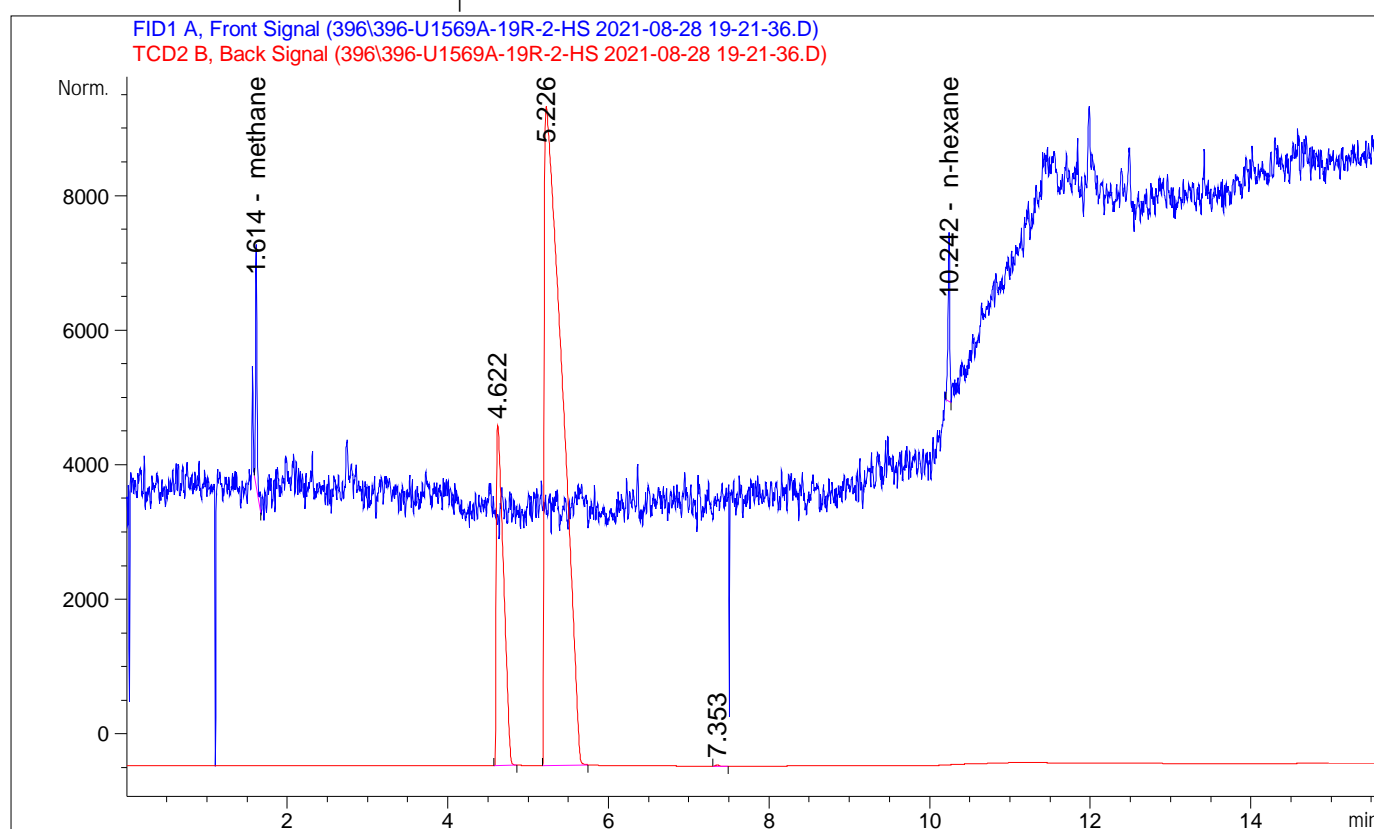

External Standard Report

```
=====
Sorted By      : Signal
Calib. Data Modified : 8/21/2021 2:01:44 PM
Multiplier     : 1.0000
Dilution       : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs
=====
```

Signal 1: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ppm]	Grp	Name
1.614	BB	1.29297e-1	9.26156	1.19749		methane
1.988		-	-	-		ethane
2.712		-	-	-		ethene
3.999		-	-	-		propane
6.334		-	-	-		propene
6.700		-	-	-		i so-butane
6.932		-	-	-		n-butane
8.505		-	-	-		i so-pentane
8.657		-	-	-		n-pentane
9.855		-	-	-		i so-hexane
10.242	BB	1.09441e-1	0.00000	0.00000		n-hexane

Totals : 1.19749

Signal 2: TCD2 B, Back Signal

RetTime [min]	Type	Area [25 µV*s]	Amt/Area	Amount [ppm]	Grp	Name
10.540		-	-	-		carbon di oxide

Totals : 0.00000

3 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

Warning : Negative results set to zero (cal. curve intercept), (n-hexane)

```
=====
Summed Peaks Report
=====
```

Signal 1: FID1 A, Front Signal

Empty table.

Signal 2: TCD2 B, Back Signal

Empty table.

```
=====
Final Summed Peaks Report
=====
```

Signal 1: FID1 A, Front Signal

Name	Total Area [25 μ V*s]	Amount [ppm]
----- ----- -----		
methane	1.29297e-1	1.1975
ethane	0.00000	0.0000
ethene	0.00000	0.0000
propane	0.00000	0.0000
propene	0.00000	0.0000
i so-butane	0.00000	0.0000
n-butane	0.00000	0.0000
i so-pentane	0.00000	0.0000
n-pentane	0.00000	0.0000
i so-hexane	0.00000	0.0000
n-hexane	1.09441e-1	0.0000

Totals : 1.1975

Signal 2: TCD2 B, Back Signal

Name	Total Area [25 μ V*s]	Amount [ppm]
----- ----- -----		
carbon di oxide	0.00000	0.0000

Totals : 0.0000

Compound-related custom fields:

*** End of Report ***