


=====

Acq. Operator	: SYSTEM	
Sample Operator	: SYSTEM	
Acq. Instrument	: NGA-2	Location : - (F)
Injection Date	: 8/24/2021 9:52:45 PM	
		Inj Volume : Manual ly
Method	: C:\CHEM32\2\METHODS\396_NGA2.M	
Last changed	: 8/23/2021 5:20:48 PM by SYSTEM	
	(modified after loading)	
Method Info	: manual headspace injections	
Sample Info	: CYL11101141	

Sample-related custom fields:

Name	Value
------	-------

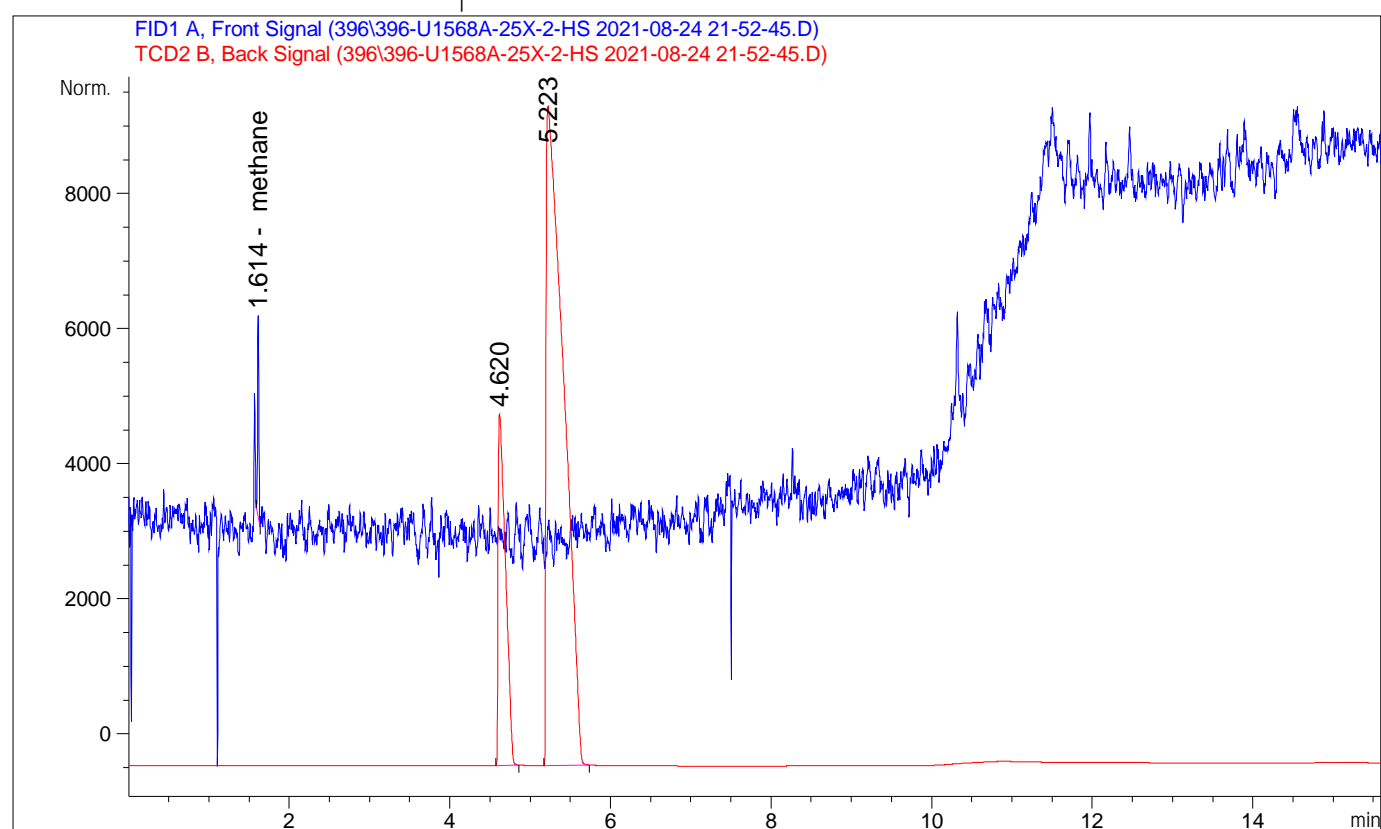

=====

External Standard Report

=====

Sorted By	: Signal
Calib. Data Modified	: 8/21/2021 2:01:44 PM
Multiplier	: 1.0000
Dilution	: 1.0000

Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ppm]	Grp	Name
1.614	BB	9.76948e-2	5.66605	5.53544e-1		methane
1.988		-	-	-		ethane
2.712		-	-	-		ethene
3.999		-	-	-		propane
6.334		-	-	-		propene
6.700		-	-	-		i so-butane
6.932		-	-	-		n-butane
8.505		-	-	-		i so-pentane
8.657		-	-	-		n-pentane
9.855		-	-	-		i so-hexane
10.020		-	-	-		n-hexane

Totals : 5.53544e-1

Signal 2: TCD2 B, Back Signal

RetTime [min]	Type	Area [25 µV*s]	Amt/Area	Amount [ppm]	Grp	Name
10.540		-	-	-		carbon di oxide

Totals : 0.00000

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

Summed Peaks Report

Signal 1: FID1 A, Front Signal

Empty table.

Signal 2: TCD2 B, Back Signal

Empty table.

Final Summed Peaks Report

Signal 1: FID1 A, Front Signal

Name	Total Area [25 μ V*s]	Amount [ppm]
----- ----- -----		
methane	9.76948e-2	0.5535
ethane	0.00000	0.0000
ethene	0.00000	0.0000
propane	0.00000	0.0000
propene	0.00000	0.0000
i so-butane	0.00000	0.0000
n-butane	0.00000	0.0000
i so-pentane	0.00000	0.0000
n-pentane	0.00000	0.0000
i so-hexane	0.00000	0.0000
n-hexane	0.00000	0.0000

Totals : 5.5354e-1

Signal 2: TCD2 B, Back Signal

Name	Total Area [25 μ V*s]	Amount [ppm]
----- ----- -----		
carbon di oxide	0.00000	0.0000

Totals : 0.0000

Compound-related custom fields:

*** End of Report ***