

Figure 1. STEMPO phantom inside the micro-CT device. The static and dynamic objects of interest inside the pipe are not visible from the outside.

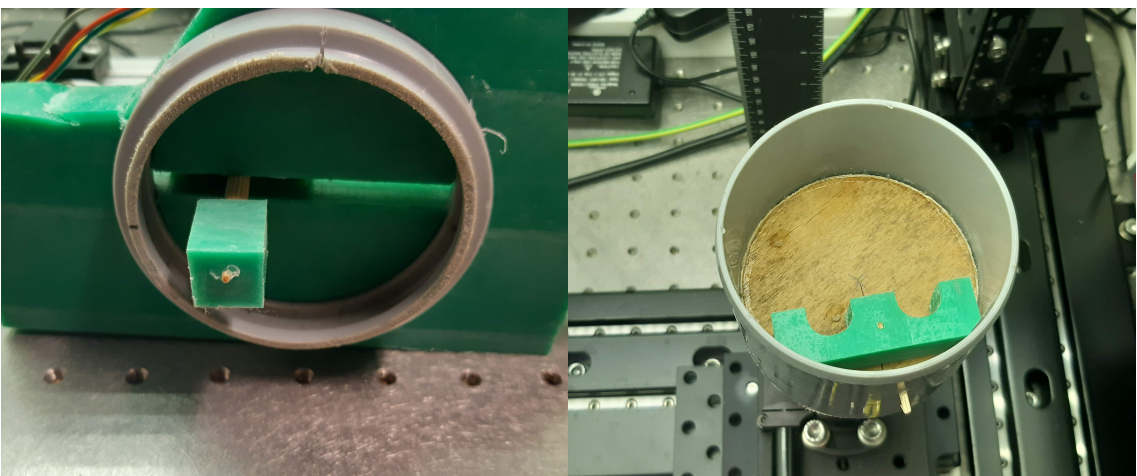


Figure 2. Interior parts of STEMPO phantom visible in the X-ray projections. On the left: moving HDPE block. On the right: boundary pipe and a static HDPE detail.